




# HP 8753C Network Analyzer

Quick Reference



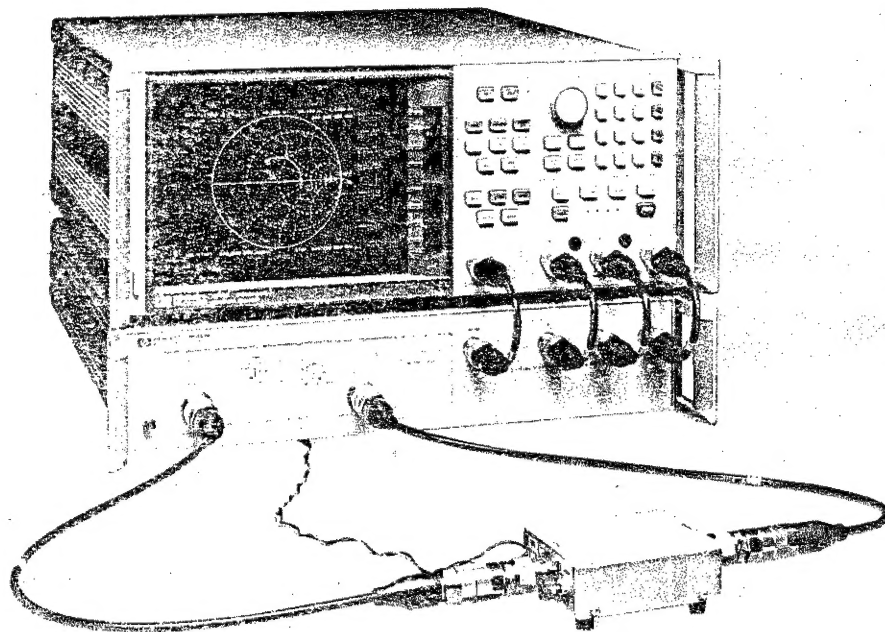

## Functional Index

Page 27  
A/R  
B/R  
S-parameters

Page 24  
Magnitude  
Phase  
Group delay  
Smith chart

Page 43  
Autoscale  
Scale  
Reference  
Electrical delay

Page 18  
Dual display  
Trace memory  
Titling

Page 9  
Averaging  
Smoothing  
IF bandwidth

Page 35  
Markers  
Marker delta

Page 12  
Calibration

Page 39  
Marker →  
Marker search  
Marker statistics

Page 29  
Power  
Trigger  
Points  
Sweep type




Page 44  
Sequencing  
Limit testing  
Transform (opt)  
6 GHz operation (opt),  
Harmonic meas (opt),  
Instrument modes

Page 16  
Plot  
Print

Page 42  
Save registers  
Clear registers  
Title registers


Page 41  
Recall registers

Page 26  
HP-IB mode  
HP-IB addresses

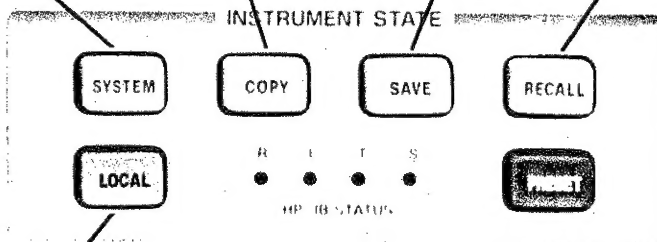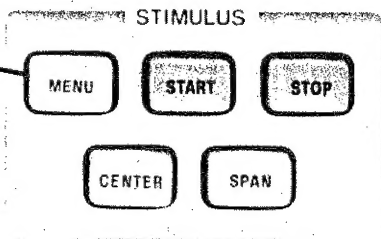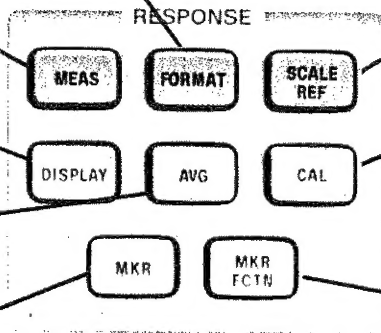

## How To Use This Book

This guide is designed to describe what the softkey menus do and to give enough information for making basic measurement decisions. A typical page of this guide, as shown below, is indexed by the front panel key, shows the keypath to the menu under discussion, and details the menu by option.

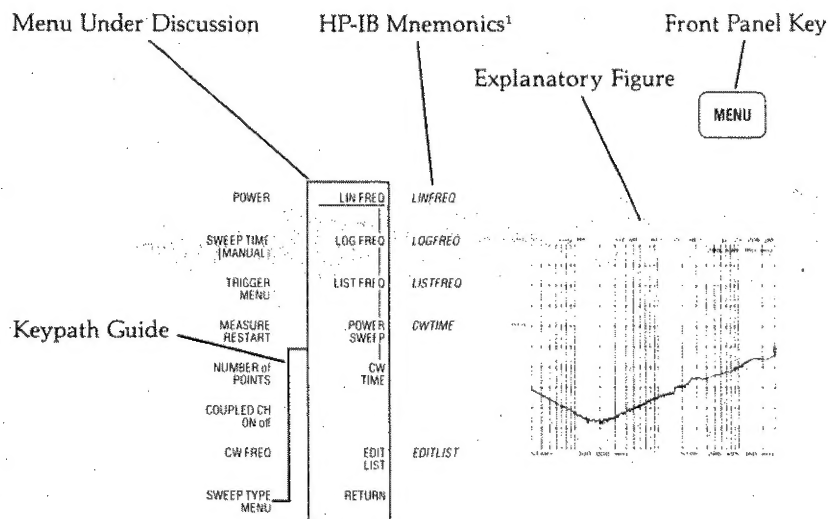


### Menu Explanation

- LIN FREQ** Activates a simple linear frequency sweep. With option 010, the analyzer can translate this data to time domain.
- LOG FREQ** Activates a logarithmic frequency sweep. The data is sampled logarithmically and displayed.
- LIST FREQ** Sweeps across the user defined frequency list. The sweep may be defined as a single segment sweep ([*SINGLE SEG SWEEP*] softkey) or an all segment sweep ([*ALL SEGS SWEEP*] softkey). The frequency list table can be entered and modified with [*EDIT LIST*].
- POWER SWEEP** Sweeps power at a single frequency. That frequency is set with [*CW FREQ*]. Power sweep is used to characterize power sensitive networks.
- CW TIME** Tunes the analyzer to a single frequency and displays the data versus time. The frequency is set with [*CW FREQ*]. With option 010 (time domain), the analyzer can translate this data to the frequency domain.
- EDIT LIST** Allows the user to create or modify the frequency list table.
- RETURN** Returns to the previous menu.

Next Menu Page 33

Next Menu Page 33

1. HP-IB is Hewlett-Packard's hardware, software, documentation, and support for IEEE 488 and IEC-625, worldwide standards for interfacing instruments.

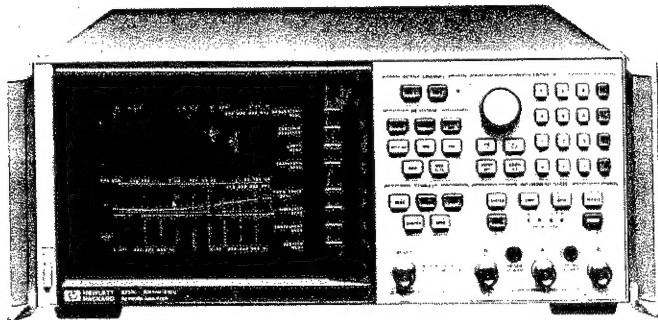

## Introduction to the HP 8753C

The HP 8753's softkey menus provide complete and flexible control of the instrument. The menus have three features that make them easy to understand and use. In situations where you can make one of several selections, the softkeys are connected by vertical lines, and the current choice underlined. In cases where a single key summarizes the selection of one of several choices, the current selection is shown in brackets below the softkey label. Lastly, the state of on/off functions is indicated below the softkey label by capitalizing either on or off.

The following is a brief introduction to the purpose of each functional key area.


### Entry

The entry area controls the value in the active entry area of the display. The step keys and the knob vary the active entry value, and the key pad enters new values. A partially entered value is indicated by the data entry arrow, which points to the last digit pressed. The units terminator keys enter the value. Any units terminator can enter any parameter, the only difference being the power of ten by which the entered value is scaled.

### Stimulus

The stimulus menu controls the microwave source. It lets you set the power, the sweep time, and the number of points. The power can range from  $-5$  to  $+20$  dBm, the sweep time from 2 msec to days, and the number of points from 3 to 1601. You can uncouple the channels so they have independent stimulus settings, and you can select the sweep type. The HP 8753 can sweep frequency linearly, logarithmically, or from an operator-defined frequency list. It can also lock onto a CW frequency and sweep time.

The [START], [STOP], [CENTER], and [SPAN] keys control the stimulus span measured. During frequency sweeps, they control frequency. During power sweeps they control power, and during time sweeps, they control time.

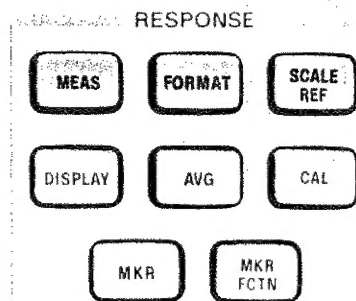

## Response

The response keys control data measurement and data processing.

**MEAS** Selects the parameter to be measured. Choose from an absolute measurement, a ratio measurement, or an S-parameter.

**FORMAT** Selects the format of the data. Display the magnitude, phase, group delay, real portion, imaginary portion, or SWR of the data, or display the data in a polar format or on a Smith chart.

**SCALE REF** Controls the size and placement of the trace on the graticule. Add a linear phase shift to the data using the electrical delay function under this key.


**DISPLAY** Controls trace memory, vector trace math, split and dual channel display, intensity, color modification, display title, and frequency blanking.

**AVG** Controls the trace noise reduction techniques. Average the data over time, reduce the IF bandwidth, or smooth a noisy trace.

**CAL** Accesses the calibration features of the analyzer. Improve the accuracy of the data by calibrating with known standards, or a power meter.

**MKR** Controls the four markers. Use the markers to read numeric values off the trace. The marker values indicate either absolute trace position, or trace position relative to a delta reference. The delta reference can be a marker, or it can be a fixed point.

**MKR FCTN** Controls the active marker functions. Use the marker position to set the stimulus parameters; use the search feature to place the marker at a specific amplitude; and use the statistics functions to characterize passband shapes and to give trace statistics.

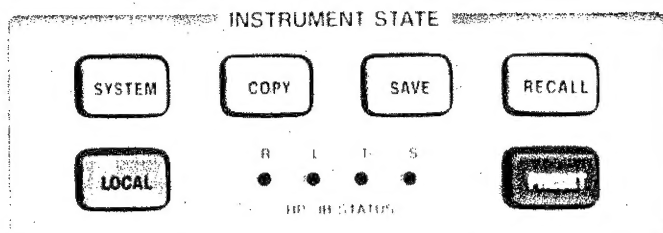

### Active Channel

The active channel keys select the active channel. Except when coupled between channels, softkey functions apply only to the active channel.

### Instrument State

The instrument state keys control functions that do not directly affect the measurement or display of data, with the exception of time domain (option 010), harmonic measurement (option 002), test sequence function, and instrument modes.

- SYSTEM** This key controls test sequencing function, harmonic measurements (option 002), limit testing, service functions, and time domain (option 010.) Time domain is a transform that calculates the impulse and step response of a device from the frequency domain information.
- COPY** Accesses the hard copy capabilities of the instrument. You can plot on an HP-GL plotter, or you can print on a compatible printer.
- SAVE** Stores, clears, and titles the save/recall registers. When a register is saved, the entire instrument state is stored. A register can be saved internally or to an external disk drive.
- RECALL** Recalls the save/recall registers. When a register is recalled, the instrument is returned to the state it was in when the register was saved.
- LOCAL** Controls the HP-IB aspects of the instrument. Select system controller mode for manual operation of the instrument, set the HP-IB address of the HP 8753, and enter the addresses of the peripherals.
- PRESET** Performs a self check, and brings the instrument back to the preset state.

## The Display


Shown here is the simplest display configuration. Turning dual channel on displays both channels at once, adding display notations for the second channel. The notations change slightly for polar and Smith chart display, the only scale information being the value at the outer circle. The marker values change also (see page 18).

## Status Notations

The status notations area of the CRT is used to show the current status of various functions for the active channel. The table below lists each notation and its meaning.

Notation	Definition
*	Instrument source or receiver parameters changed since last complete sweep.
↑	Trace in progress.
Hld	Trace is in hold.
tsH	Trace is in hold due to test set limitation.
ext	Waiting for external trigger.
man	Waiting for a manual trigger.
Gat	Gating is on (see option 010, time domain).
P↓	Source power output has tripped.
P?	ALC is unlevelled at start of sweep.
PC	Power meter calibration is on.
PC?	Power meter calibration requires 8753 source power outside its normal range.
PCo	Power changed since last power meter calibration.
Cor.	Error correction is on.
C?	Error correction is on but questionable. Caused by interpolation — change in power sweep time, or IF bandwidth.
C2	2-port error correction is on, but updating only two of the four S-parameters.
C2?	2-port error correction is on but questionable.
Avg	Trace averaging is on.
(Avg)	Number displaying averaging factor.
Smo	Trace smoothing is on.
H=2	Second harmonic of source is being measured.
H=3	Third harmonic of source is being measured.
Ofs	Frequency offset mode is on.
Of?	Source offset in question.
x2	85047A is in 6 GHz range.
x2?	85047A is in 6 GHz range, but the power has been changed from default.
Del	Electrical delay or phase offset has been added in.



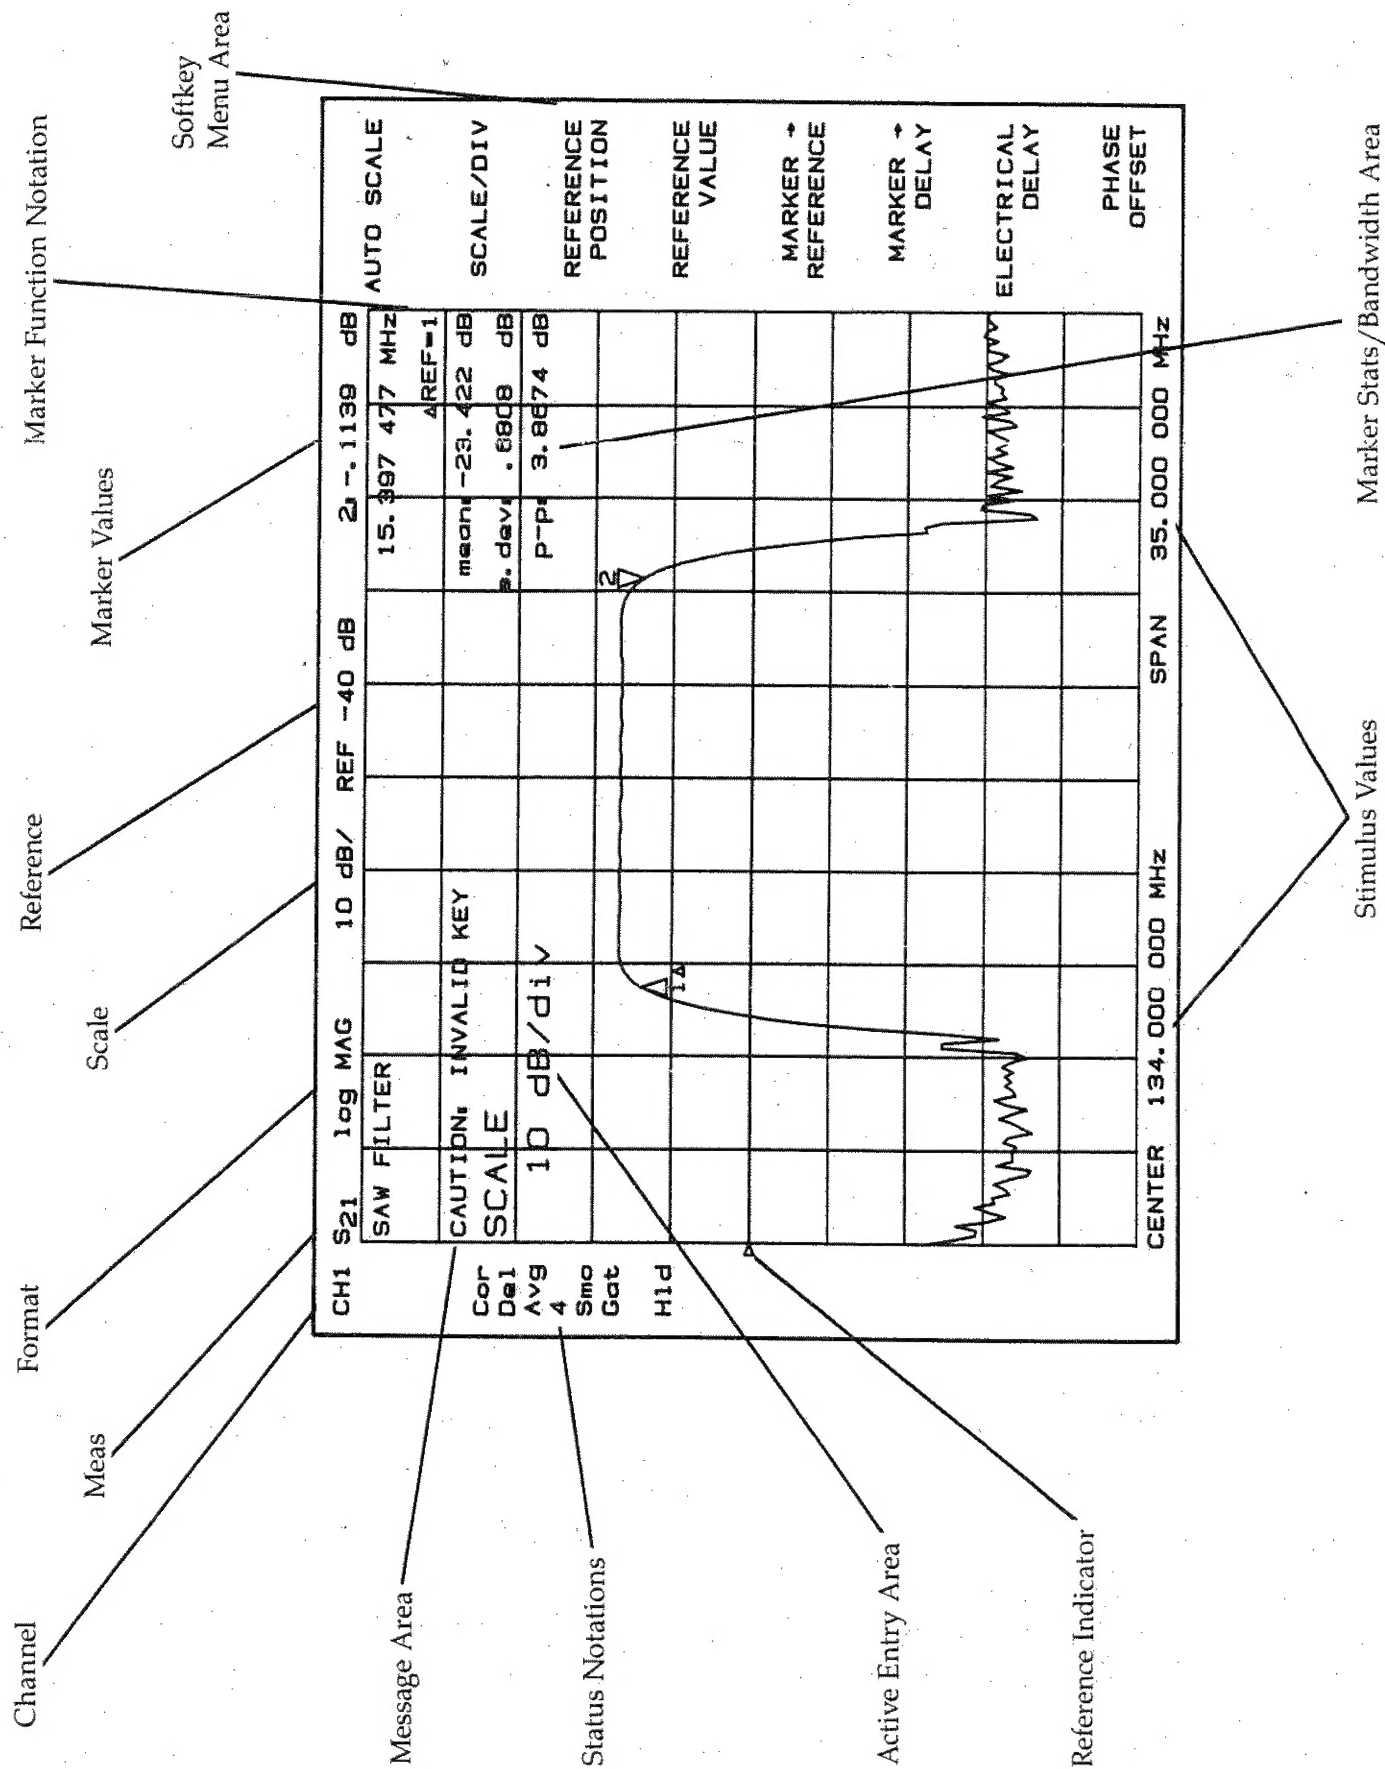



## Common Warning Messages

... CHANGE HP-IB to SYST CONT or PASS CONTROL

HP-IB control is needed before a plot, print, or disk access. See page 26.

## CORRECTION TURNED OFF

The measurement state was changed, so correction was turned off. See page 10.

OVERLOAD ON INPUT [R,A,B], POWER REDUCED

The power at an input exceeded safety levels, so the RF source power was reduced.

Power can be restored by turning power trip off. See page 30.

SOURCE PARAMETERS CHANGED



When error correction was turned on, the stimulus state of the last calibration was recalled, or source frequency exceeds allowed range in frequency offset or harmonic measurements mode. See page 10.

☐ SWEEP TIME INCREASED

The entered sweep time was too fast for the current measurement. Sweep time increased to the minimum possible time.

1  
1  
1  
1  
.  
.  
i  
t  
e  
v  
J  
C  
r  
e  
t  
g  
7  
r  
i  
t  
f  
V  
t  
c  
8

AVG

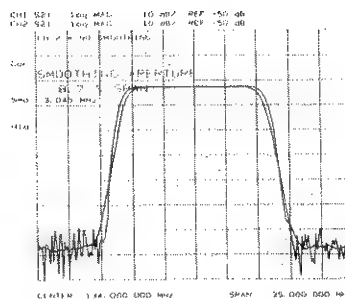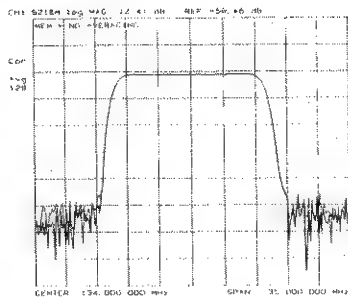

## Reducing Trace Noise

The HP 8753 has three functions that help reduce the effect of noise on the data: averaging, variable IF bandwidth, and smoothing.

Both averaging and IF bandwidth increase sensitivity to coherent signals. Averaging reduces random noise by averaging the vector data from sweep to sweep. Narrowing the IF bandwidth reduces the amount of noise measured. Smoothing, on the other hand, filters the displayed trace, making noisy data more readable.

### Averaging

The HP 8753 uses an exponentially weighted running vector average for IF averaging. The weight is one over the effective averaging factor. The effective averaging factor is displayed under the Avg notation. It begins at 1, and counts up to the user entered averaging factor, incrementing once per sweep. The noise is reduced, often visibly, with each new sweep as the effective averaging factor increments.

### IF Bandwidth

The IF bandwidth is the effective receiver bandwidth. Reducing the IF bandwidth reduces the noise that is measured during the sweep, but also may slow down the sweep. While averaging requires multiple sweeps to reduce noise, narrowing the IF bandwidth reduces the noise on every sweep.


### Smoothing

The HP 8753 uses a linear block moving average to smooth the trace. The effect is to remove sharp edges from the trace, much like video filtering. The smoothing aperture is the width of the linear block average that is moved across the trace. Larger apertures smooth out the trace more, reducing the resolution with which individual trace features can be resolved.

When measuring group delay, smoothing is used to increase the group delay aperture. The smoothing aperture becomes the group delay aperture when smoothing is on.


AVG

AVERAGING RESTART	AVERREST
AVERAGING FACTOR	AVERFACT
AVERAGING on OFF	AVERON, AVEROFF
SMOOTHING APERTURE	SMOOPER
SMOOTHING on OFF	SMOON, SMOOFF
IF BW [3000 Hz]	IFBW

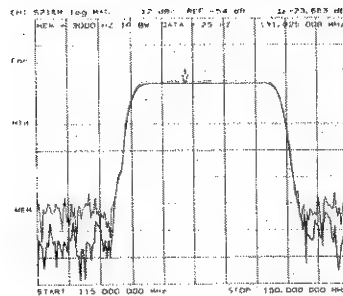

- AVERAGING RESTART** Clears the average and restarts it with the next sweep.
- AVERAGING FACTOR** Enters the averaging factor. The effective averaging factor appears under the Avg notation. It will count up to the entered averaging factor and stop, indicating that the displayed trace has reached the desired level of averaging.
- AVERAGING on OFF** Averages each new sweep into the trace, reducing random noise over time. The Avg notation comes on.
- SMOOTHING APERTURE** Specifies the percent of the trace that is to be used as the smoothing aperture. The equivalent aperture in the current stimulus units is noted below the active entry area. A narrow aperture allows finer detail.
- SMOOTHING on OFF** Smooths the displayed trace, much like video filtering. Turns on the Smo notation.
- IF BW [3000 Hz]** Sets the IF bandwidth. A narrow bandwidth reduces the noise floor but may slow down the sweep speed.

CAL

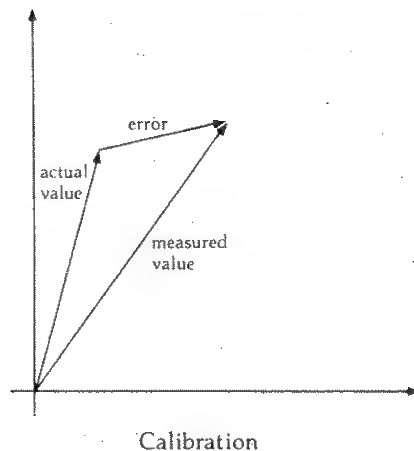

### Measurement Calibration

Accuracy in network analysis is greatly influenced by the measurement system. Parts of the measurement setup such as interconnecting cables and adapters (as well as the instrument itself) all introduce variations in magnitude and phase that can mask the actual performance of the DUT.


The calibration step effectively characterizes and removes the effects of repeatable measurement variations in the test system. The "systematic errors" with which the calibration step is concerned are:

- Frequency Response (Tracking)
- Leakages (Directivity and Crosstalk)
- Mismatches (Source Match and Load Match)

The HP 8753 has several methods of measuring and compensating for these test system imperfections. Each method utilizes the measurement of standard devices and specific equations (error models) to remove one or more of the systematic errors mentioned above. By applying the data obtained from the standards to a specific error model, the calibration step is able to characterize the measurement system and thus increase the accuracy (by reducing the uncertainty) of the DUT's measurement results. The accuracy of the calibration step is dependent on the quality of the standards used for calibrating. Since calibration standards are very precise, excellent accuracy enhancement is achieved.

Calibrations are valid only for a specific stimulus state. The stimulus state is the frequency range, number of points, sweep time, output power, and sweep type. Changing the stimulus state with correction on causes a warning. If the calibration is invalidated, correction is turned off. Pressing [INTERPOL on OFF] will allow you to increase the number of points, or decrease frequency range without losing calibration. However, this mode is unspecified and a C? will appear. If the calibration is simply in question, as when sweep time is changed, the status notation changes to C?. Turning correction on recalls the stimulus state for that calibration.

The HP 8753C has default definitions for the HP 8753C calibration kits, stored by connector type. A calibration kit definition is a set of the key characteristics of the standards that the analyzer uses to calculate the calibration data. The operator can select a default kit using [CAL KIT], and can modify the current definition using [MODIFY CAL KIT].

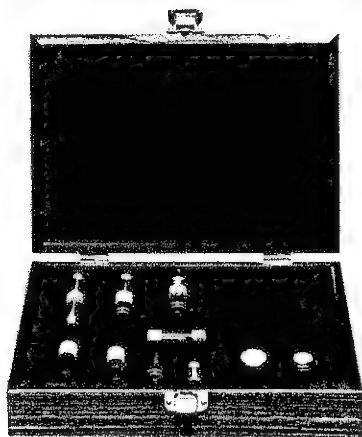

CAL

Below are listed the measurement errors that the HP 8753C calibrations will correct.

### **Transmission and Reflection Frequency Response.**

Frequency response is the simplest error correction. The calibration standard for reflection is either a short or an open, and for transmission is a "thru". In correcting for frequency response, the analyzer also corrects for differences in path length and attenuation between the measurement channels. All calibrations correct for frequency response.

### **Directivity**

In a reflection measurement, it is necessary to separate the forward traveling signal from the reflected signal. The relative leakage of the forward signal into the reflected signal is characterized by directivity. The calibration standard for measuring directivity is a load. All calibrations, except response, correct for directivity.

### **Crosstalk (Isolation)**

Signal leakage from one test port to the other represents a source of measurement error. The calibration for isolation is done by terminating the ports and measuring the signal leaking between the RF paths. Isolation is an option in the response/isolation and 2-port calibrations.

### **Source Match**

If the output measurement port is not precisely the characteristic impedance of the measurement system (50 ohms), undesired reflections result. To remove such reflections, the source match is calculated from the responses of a short, an open, and a load. The 1-port and 2-port calibrations correct for source match.

### **Load Match**

The same problem as source match, but referring to the input port. The full 2-port calibration corrects for load match.

**NOTE:** By convention, when the connector sex is provided in parentheses for a calibration standard, it refers to the sex of the test port connector, not the actual standard. For example, short (m) indicates that the test port connector (or cable or adapter), not the short circuit connector, is male.

## CAL

CORRECTION  
on OFF

INTERPOL  
on OFF

CALIBRATE  
MENU

RESUME CAL  
SEQUENCE

CAL KIT  
[7 mm]


PWRMTR CAL  
[off]

MORE

CORR ON  
CORROFF

COR ON  
COR OFF

RESC

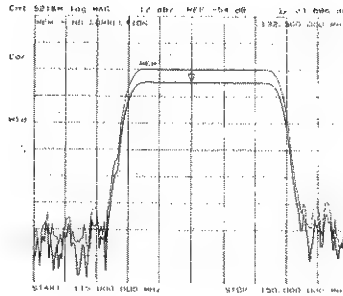

CORRECTION  
on OFF

Turns on error correction. The analyzer uses the most recent calibration data for the parameter being displayed. If the stimulus state has been changed since calibration, the state is recalled. Turns on the Cor notation.

INTERPOL  
on OFF

Allows you to change the number of points or decrease the frequency range of a measurement without losing calibration.

CALIBRATE  
MENU

Performs a new calibration. Correction is automatically turned on at the completion of the calibration sequence.

*Next Menu Page 13*

RESUME CAL  
SEQUENCE

If a calibration sequence was interrupted, this softkey allows the user to re-enter the sequence at the point of exit.

CAL KIT  
[7 mm]

Allows the operator to select a default calibration kit or modify the current kit. Calibration kits hold the characteristics of the calibration standards. The defaults are called up by connector type, and are for the standard HP 8753C calibration kits.

PWRMTR CAL  
[OFF]

Enables you to use an external power meter to normalize the output power of the internal source with respect to an external measurement port.


MORE

Leads to the calibration parameter menu.

*Next Menu Page 15*



# CAL

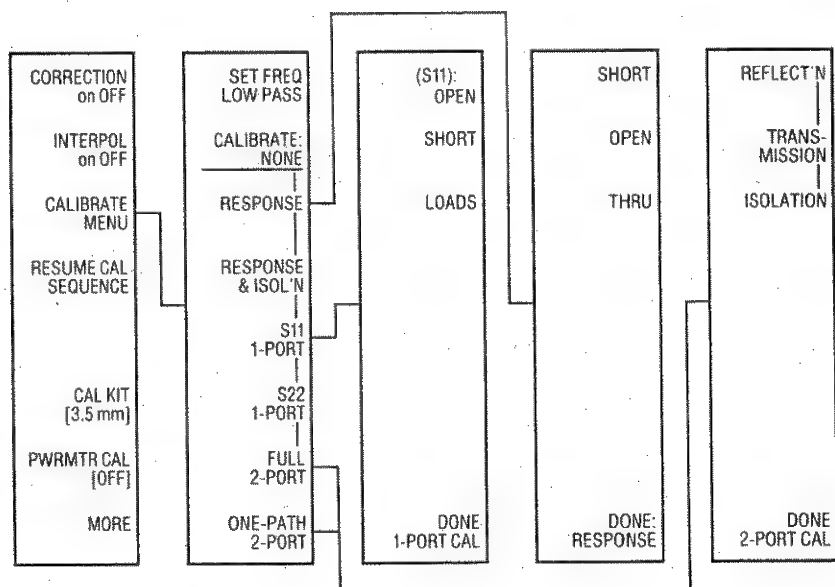

**SET FREQ LOW PASS** Changes the frequency sweep to accommodate time domain low pass mode (option 010). If this mode is used, the frequencies must be set before calibration.

**CALIBRATE: NONE**

**RESPONSE** Corrects for frequency response as described on page 11. Requires only one standard, using either an open or a short for reflection, or a "thru" for transmission.

**RESPONSE & ISOL'N** In transmission, corrects for frequency response and isolation errors. In reflection, corrects for frequency response and directivity errors. Requires two standards.


**S11 1-PORT** Corrects for frequency response, directivity, and source match errors from port 1 reflection measurements. Requires three standards.

**S22 1-PORT** Same as S11 1-port, but for port 2.

**FULL 2-PORT** A full correction for all the errors on page 11, in both the forward and reverse directions.

**ONE-PATH 2-PORT** A full correction for all the errors on page 11, but does not require an S-parameter test set. The operator has to manually reverse the device and retrigger each sweep. [SINGLE SWEEP] will also retrigger the sweep.

**CAL**

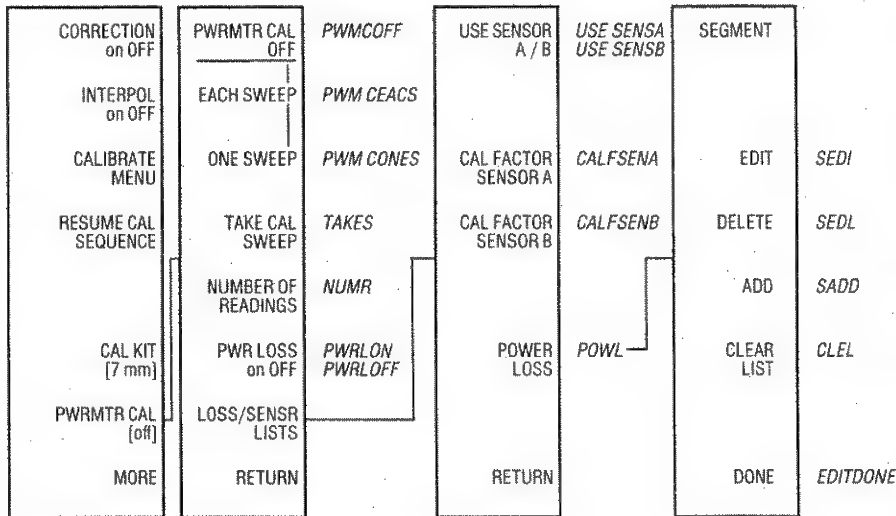

<b>PWRMTR CAL</b>	Controls correction after the calibration data has been taken.
<b>OFF</b>	When the normalization is on, the CAL POWER active function is the power at the power meter plus any specified power loss, not the power at the analyzer's output. Turns on PC notation.

**EACH SWEEP** Sets up the instrument to take calibration data every sweep. This method of calibration is very accurate, but slow.

**ONE SWEEP** Sets up the analyzer to take one sweep of calibration data and use it to set up a table. This table is used as a reference from that point forward until another calibration sweep is taken.

<b>TAKE CAL SWEEP</b>	Initiates the sweep of calibration data. Turns power meter cal on.
-----------------------	--



**NUMBER OF READINGS** Defines the number of readings to be taken at every frequency. To achieve higher accuracy increase the number of readings.

**PWR LOSS** This offsets the readings of the power meter.  
*on OFF*

<b>LOSS/SENSR</b>	Leads to a menu containing lists of power loss and sensor vs.
<b>LIST</b>	frequency data.

**RETURN** Returns to the previous menu.

CAL

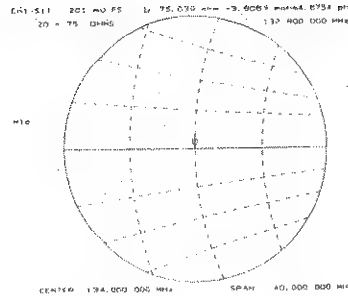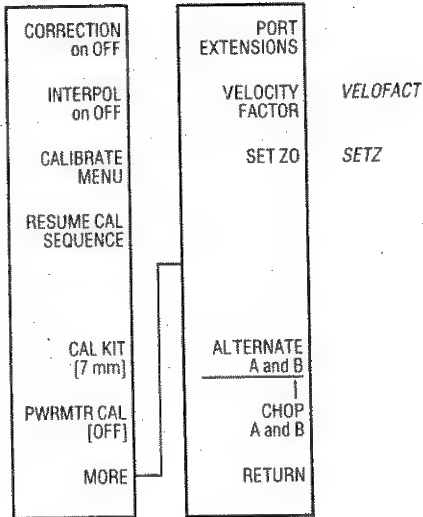


- PORT EXTENSIONS** Allows the user to enter the reference plane extensions for inputs A and B and ports 1 and 2. Extends the apparent reference plane to the end of the port extensions.
- VELOCITY FACTOR** Enters the velocity factor that the HP 8753C uses to calculate equivalent electrical length.
- SET Z0** Sets the characteristic impedance used in calculating measured impedance.
- ALTERNATE A and B** Alternately samples channels while performing a measurement.
- CHOP A and B** Simultaneously samples channels allowing simultaneous measurements of  $S_{11}$  and  $S_{21}$ .
- RETURN** Returns to the previous menu.



COPY


PRINT [STANDARD]	PLOT DATA ON off	PDATAON, PDATAOFF
PLOT	PLOT MEM ON off	PMEMON, PMEMOFF
SELECT QUADRANT	PLOT GRAT ON off	PGRATON, PGRATOFF
DEFINE PLOT	PLOT TEXT ON off	PTEXTON, PTEXTOFF
CONFIGURE PLOT	PLOT MKR ON off	PMKRON, PMKROFF
PRINT/PLOT SETUPS	SCALE PLOT [FULL]	SCAPFULL, SCAPGRAT
LIST VALUES	PLOT SPEED [FAST]	PLOSSLOW, PLOSFAST
OP PARAM (MKRS ETC.)	RETURN	

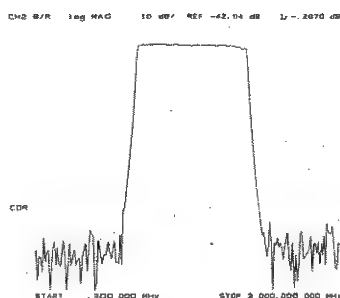

- PLOT DATA** ON off Includes the data trace on the plot.
- PLOT MEM** ON off Includes the memory trace on the plot.
- PLOT GRAT** ON off Includes the graticule on the plot.
- PLOT TEXT** ON off Includes all of the display text on the plot, except for the marker values, frequency list table, and limits table.
- PLOT MKR** ON off Plots the markers and their values visible on the CRT.
- SCALE PLOT** [FULL] [FULL] is the normal plot mode. [GRAT] expands the graticule to fill the plot area as defined by P1 and P2. Allows plotting on printed forms.
- PLOT SPEED** [FAST] [FAST] Changes between normal plotting at [FAST] speed, and low speed plotting at [SLOW] speed for transparencies.
- RETURN** Returns to the previous menu.

## DISPLAY

DUAL CHAN on OFF	DUACON, DUACOFF
DISPLAY: DATA	DISPDATA
MEMORY	DISPMEMO
DATA and MEMORY	DISPDATM
DATA/MEM	DISPDMM
DATA-MEM	DISPDM
DATA → MEMORY	DATI
MORE	

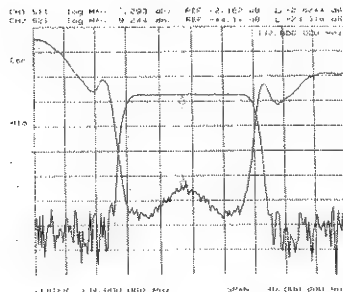


- DUAL CHAN on OFF** Displays both channels at once. They will be placed on separate graticules if split display mode (page 19) is on.
- DISPLAY: DATA** Displays the current data.
- MEMORY** Displays the trace memory of the active channel, using the current display format, scale, and reference. Works only if compatible data has been stored in memory.
- DATA and MEMORY** Displays both the current data and memory traces, with identical scaling and format.
- DATA/MEM** Vector trace math. Divides the data by memory, normalizing the data to the memory. The math is performed on the linear data, before display formatting.
- DATA-MEM** Subtracts the memory from the data. The vector subtraction is performed on the linear data, before display formatting.
- DATA → MEMORY** Stores the active trace in the memory of the active channel.
- MORE** Leads to more display choices.

Next Menu Page 19


## DISPLAY

DUAL CHAN on OFF	SPLIT DISP ON off
DISPLAY: DATA	BEEP DONE ON off
MEMORY	BEEP WARN on OFF
DATA AND MEMORY	ADJUST DISPLAY
DATA/MEM	TITLE
DATA-MEM	D2/D1 to D2 on OFF
DATA → MEMORY	FREQUENCY BLANK
MORE	RETURN

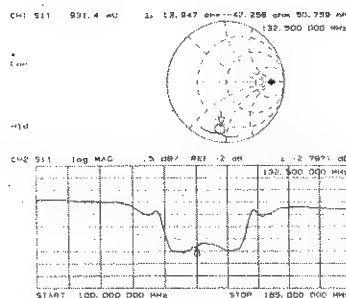

- SPLIT DISP**  
*ON off* Displays each channel on a separate graticule when dual channel mode (previous page) is on.
- BEEP DONE**  
*ON off* Sounds the beeper whenever the analyzer finishes certain functions, such as data to memory, measuring a calibration standard, or saving an instrument state.
- BEEP WARN**  
*on OFF* Sounds the beeper when a warning message is displayed.
- ADJUST DISPLAY** Leads to the "Adjust Display" menu (page 20).
- TITLE** Leads to the "Title" menu (page 22).
- D2/D1 to D2**  
*on OFF* Displays on channel 2 the data of channel 2 divided by the data of channel 1, when ON (preset state shown).
- FREQUENCY BLANK** Prevents display of frequency information.
- RETURN** Returns to the "Display" menu (page 18).

## DISPLAY

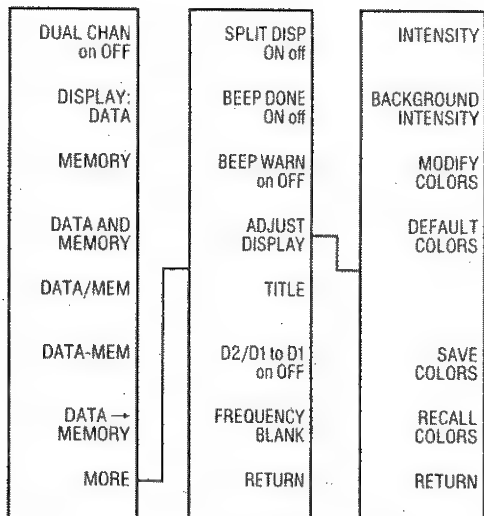

**INTENSITY** Sets the CRT intensity as a percentage of the brightest setting. The factory-set default value is stored in non-volatile memory.

**BACKGROUND INTENSITY** As above for the background.

**MODIFY COLORS** Leads to the color modification menu (see page 21)

**DEFAULT COLORS** Returns all color settings to the factory-set default values.

**SAVE COLORS** Saves the modified version of the color set.

**RECALL COLORS** Recalls previously saved color sets (if any).

**RETURN** Returns to the "Display More" menu (page 19).



# **DISPLAY**


[MORE]

SPLIT DISP ON off	INTENSITY	CH1 DATA LIMIT LN
BEEP DONE ON off	BACKGROUND INTENSITY	CH1 MEM
BEEP WARN on OFF	MODIFY COLORS	CH2 DATA LIMIT LN
ADJUST DISPLAY	DEFAULT COLORS	CH2 MEM
TITLE		GRATICULE TEXT
D2/D1 to D2 on OFF	SAVE COLORS	WARNING
FREQUENCY BLANK	RECALL COLORS	TEXT
RETURN	RETURN	RETURN

Note: these keys (except return) lead to a second color menu that allows modification of tint, brightness, and color. If varying tint has no visible effect, increase the color percentage first.

<b>CH1 DATA LIMIT LN</b>	Selects channel 1 data trace and limit line for color modification.
<b>CH1 MEM</b>	Selects channel 1 memory trace for color modification.
<b>CH2 DATA LIMIT LN</b>	Selects channel 2 data trace and limit line for color modification.
<b>CH2 MEM</b>	Selects channel 2 memory trace and reference line for color modification.
<b>GRATICULE TEXT</b>	Selects the graticule and some softkey text for color modification.
<b>WARNING</b>	Selects the warning annotation (like error messages) for color modification.
<b>TEXT</b>	Selects all non-data text (for example, "operating parameters") for color modification.
<b>RETURN</b>	Returns to the "Adjust Display" menu (page 20).

## DISPLAY

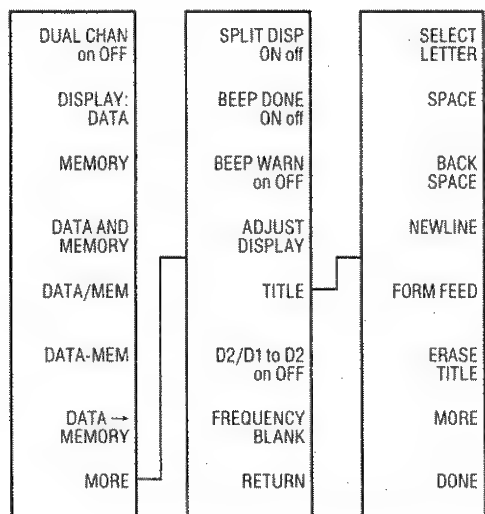

**SELECT LETTER** Adds the character above the cursor to the title.

**SPACE** Adds a space (as between words) to the title.

**BACK SPACE** Deletes the last character (or space) from the title.

**NEWLINE** Adds the symbol [NL] to the title. In test sequencing mode, it is sent as a command to a HP-IB controllable device (such as a printer).

**FORM FEED** The symbol is [FF]; otherwise same as above.


**ERASE TITLE** Erases the title displayed.

**MORE** Leads to the "Title More" menu (page 23).

**DONE** Returns to the "Display More" menu (page 19).

**DISPLAY**

**[MORE]**

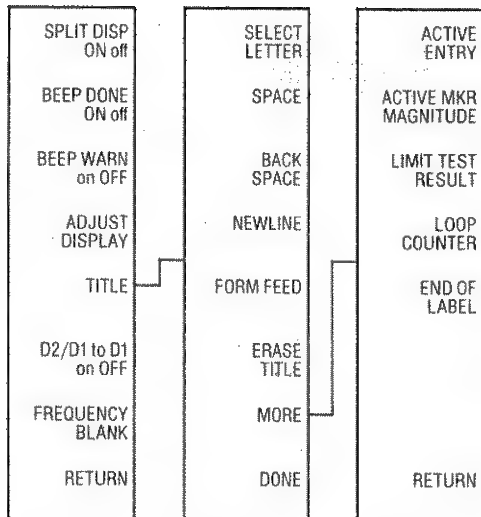

These keys cause the named data to be printed out with the title. For details see chapter 13 of the Reference section.

**ACTIVE ENTRY** Prints the name of the active entry.

**ACTIVE MKR MAGNITUDE** Prints the active marker amplitude.



**LIMIT TEST RESULT** Prints the result of a limit test.

**LOOP COUNTER** Prints the current value of the loop counter.

**END OF LABEL** Terminates the HP-GL "LB" (label) command.

**RETURN** Returns to "Title" menu (page 22)

## FORMAT

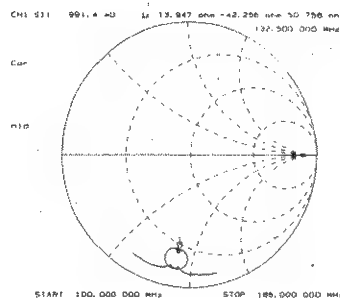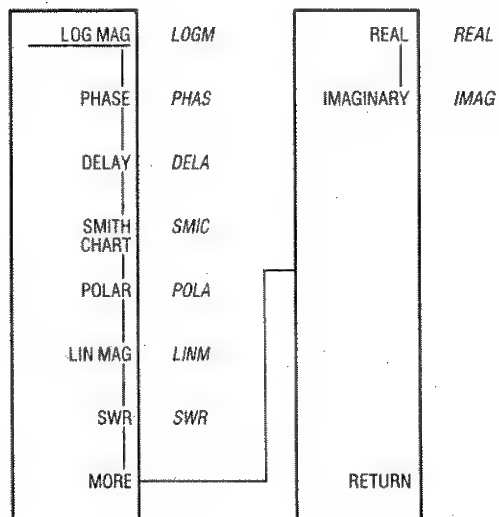

**LOG MAG** Displays the log magnitude of the data in dB.

**PHASE** Displays the phase portion of the data in degrees.

**DELAY** Displays group delay. Group delay is the derivative of phase with respect to frequency. Since the aperture is the frequency step, it will vary across log and list frequency sweeps. Smoothing can increase the aperture.

**SMITH CHART** Displays the data on a Smith chart. There are special marker modes for this format. See page 37.

**POLAR** Displays the data in a polar format. There are special marker modes for this format. See page 37.

**LIN MAG** Displays the linear magnitude of the data.

**SWR** Displays the data formatted into SWR.

**MORE** Leads to more display choices.

LOCAL

The analyzer can control certain peripheral devices over HP-IB, namely compatible printers, plotters and disk drives. It also allows other devices to control the same peripherals and the analyzer itself. Because of possible conflicts arising over peripheral control, the analyzer has three different HP-IB modes.

### **System Controller**

If the you want the analyzer to take control of the peripherals and there are no other active controller devices on the bus, put the it in system controller mode. This is the mode intended for manual operation.

### **Talker/Listener**


This mode allows an external controller to command the analyzer to access peripherals. In this mode, the controller coordinates all bus activity. This is the normal program control mode.

### **Pass Control**

If another active controller is present, pass control mode allows you to request a plot, print, or disk storage from the front panel. In order for this mode to operate, the external controller must detect the analyzer's request for control, and then pass control it. When the transmission is complete, the analyzer will pass control back.

## MEAS

Ref: FWD S11 (A/R)	S11
Trans: FWD S21 (B/R)	S21
Trans: REV S12 (B/R)	S12
Ref: REV S22 (A/R)	S22
ANALOG IN Aux Input	ANAL
CONVERSION [OFF]	
INPUT PORTS	

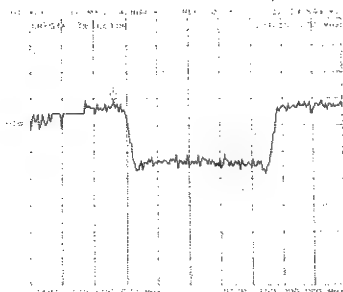

### Ref: FWD S11 (A/R)

Configures the S-parameter test set so that A/R measures S11, and annotates the display as S11. If no S-parameter test set is present, the analyzer will measure A/R and annotate the display as S11.

### Trans: FWD S21 (B/R)

Configures the S-parameter test set so that B/R measures S21, and annotates the display as S21. If no S-parameter test set is present, the analyzer will measure B/R and annotate the display as S21.

### Trans: REV S12 (A/R)

Configures the S-parameter test set so that A/R measures S12, and annotates the display as S12. If there is no S-parameter test set present, then the analyzer measures B/R and annotates the display as S12.

### Ref: REV S22 (B/R)

Configures the S-parameter test set so that B/R measures S22, and annotates the display as S22. If there is no S-parameter test set present, then the analyzer measures A/R and annotates the display as S22.

### ANALOG IN Aux Input

Measures the signal at the rear panel AUX INPUT. Also has service functions.

### CONVERSION [OFF]


Formats the data as impedance, admittance, or inverted S-parameters.

### INPUT PORTS

Brings up the port measurement menu.

# MEAS

A/R	AR
B/R	BR
A/B	AB
A	MEASA
B	MEASB
R	MEASR
CONVERSION [OFF]	
S PARAMETERS	

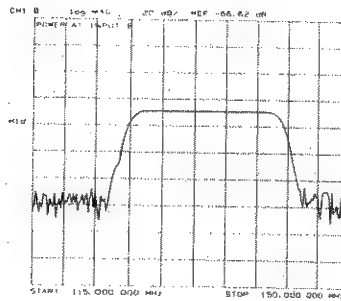

**A/R** Measures the ratio of input A to input R.

**B/R** Measures the ratio of input B to input R.

**A/B** Measures the ratio of input A to input B.

**A** Measures the signal at input A.

**B** Measures the signal at input B.

**R** Measures the signal at input R.


**CONVERSION [OFF]** Formats the data as transmittance, admittance, or inverted S-parameters instead of S-parameters.

**S  
PARAMETERS** Brings up the S-parameter menu.

Next Menu page 28

## MEAS

Ref: FWD S11 (A/R)	S11
Trans: FWD S21 (B/R)	S21
Trans: REV S12 (B/R)	S12
Ref: REV S22 (A/R)	S22
ANALOG IN Aux Input	ANA/
CONVERSION [OFF]	
INPUT PORTS	

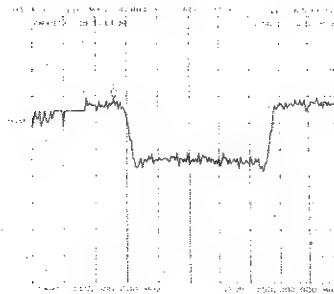

### Ref: FWD S11 (A/R)

Configures the S-parameter test set so that A/R measures S11, and annotates the display as S11. If no S-parameter test set is present, the analyzer will measure A/R and annotate the display as S11.

### Trans: FWD S21 (B/R)

Configures the S-parameter test set so that B/R measures S21, and annotates the display as S21. If no S-parameter test set is present, the analyzer will measure B/R and annotate the display as S21.

### Trans: REV S12 (A/R)

Configures the S-parameter test set so that A/R measures S12, and annotates the display as S12. If there is no S-parameter test set present, then the analyzer measures B/R and annotates the display as S12.

### Ref: REV S22 (B/R)

Configures the S-parameter test set so that B/R measures S22, and annotates the display as S22. If there is no S-parameter test set present, then the analyzer measures A/R and annotates the display as S22.

### ANALOG IN Aux Input

Measures the signal at the rear panel AUX INPUT. Also has service functions.

### CONVERSION [OFF]

Formats the data as impedance, admittance, or inverted S-parameters.


### INPUT PORTS

Brings up the port measurement menu.



# MENU

POWER	POWE
SWEEP TIME [MANUAL]	SWET
TRIGGER MENU	SWEA
NUMBER OF POINTS	
MEASURE RESTART	POIN
COUPLED CH ON off	COUCON, COUCOFF
CW FREQ	CWFREQ
SWEEP TYPE MENU	

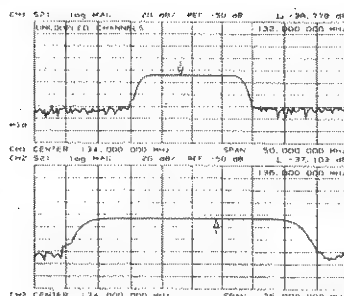

**POWER** Leads to the power menu, which controls the output power and slope compensation, and the attenuators in S-parameter test sets.

*Next Menu Page 30*

**SWEEP TIME [MANUAL]** Sets manual control of the sweep time. The actual sweep time may increase from the entered sweep time as more functions are activated. Entering a value of zero will set this to AUTO mode where the sweep time will be set to the minimum possible value.

**TRIGGER MENU** Leads to the sweep trigger menu.

*Next Menu Page 31*

**NUMBER of POINTS** Enters the number of data points per trace, ranging from 3 to 1601. A greater number of points gives greater data density, but slows the sweep and requires more memory for saving instrument states and performing calibrations.

**MEASURE RESTART** Restarts the sweep. If a 2-port calibration is active, the forward and reverse parameters are measured.

**COUPLED CH ON off** Locks both channels into the same stimulus values. Uncoupled channels cause the analyzer to alternate between the two sets of stimulus values.


**CW FREQ** Sets the frequency for CW time sweep, or power sweep.

**SWEEP TYPE MENU** Leads to the sweep type menu.

*Next Menu Page 32*

## MENU

POWER	POWER	POWE
SWEEP TIME [MANUAL]	SLOPE	SLOPE
TRIGGER MENU	SLOPE on OFF	SLOPON, SLOPOFF
NUMBER of POINTS	POWER TRIP on OFF	POWTON, POWTOFF
MEASURE RESTART	ATTENUATOR PORT 1	ATTP1
COUPLED CH ON off	ATTENUATOR PORT 2	ATTP2
CW FREQ	COUPLE PWR ON off	COUP
SWEEP TYPE MENU	RETURN	

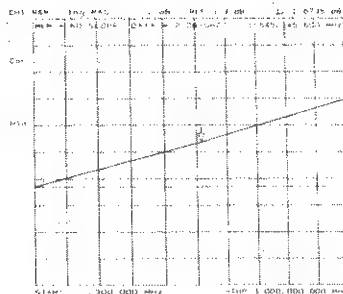

**POWER** Sets the RF source power.

**SLOPE** Enters the desired increase in RF power per GHz of sweep.

**SLOPE on OFF** Increases the output power with frequency, the sweep starting at the selected power level and increasing with the entered slope value. Counteracts frequency related losses. Calibrate with slope on if it is to be used.

**POWER TRIP on OFF** When on, an overload condition was detected on one of the inputs and power was reduced to its minimum level. Turning trip off restores the power level with the [POWER] key.

**ATTENUATOR PORT 1** Controls the port 1 programmable attenuator in the S-parameter test set.

**ATTENUATOR PORT 2** Controls the port 2 programmable attenuator in the S-parameter test set.

**COUPLE PWR ON off** When this function is on, the power between channels is coupled. When this function is off, the power between channels is uncoupled.

**RETURN** Returns to the previous menu.

# MENU

POWER	HOLD	HOLD
SWEEP TIME	SINGLE	SING
TRIGGER MENU	NUMBER of GROUPS	NUMG
NUMBER of POINTS	CONTINUOUS	CONT
MEASURE RESTART	TRIGGER TRIG OFF	EXTTOFF
COUPLED CH ON off	EXT TRIG on SWEEP	EXTTON
CW FREQ	EXT TRIG on POINT	EXTTPOIN
SWEEP TYPE MENU	MANUAL TRG on POINT	MANTRIG

**HOLD** Stops updating the sweep.

**SINGLE** Executes a single sweep, and then goes into hold.

**NUMBER of GROUPS** Executes the entered number of groups, and then goes into hold. Measuring a group updates an error corrected trace once, which, depending on the calibration used, may entail more than one sweep.

**CONTINUOUS** Continuously updates the sweep.


**TRIGGER TRIG OFF** Triggers the analyzer's sweep off the rear panel EXTERNAL TRIGGER input.

**EXT TRIG on SWEEP** Enables an external source to trigger an entire sweep.

**EXT TRIG on POINT** Enables an external source to trigger a sweep point by point.

**MANUAL TRG on POINT** Enables the user to trigger a sweep from the HP 8753's front panel.

## MENU

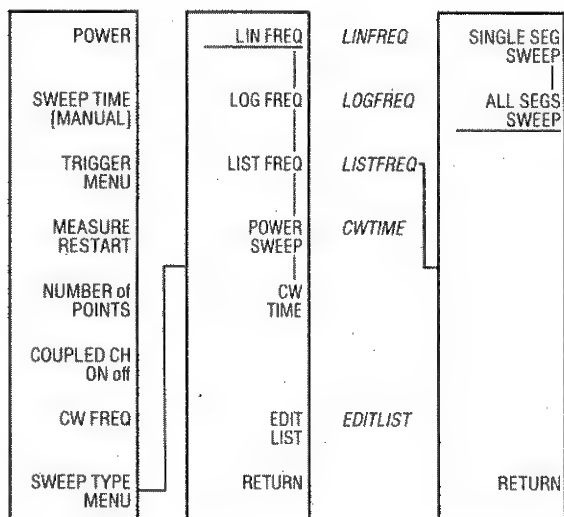

**LIN FREQ** Activates a simple linear frequency sweep. With option 010, the analyzer can translate this data to time domain.

**LOG FREQ** Activates a logarithmic frequency sweep. The data is sampled logarithmically and displayed.

**LIST FREQ** Sweeps across the user defined frequency list. The sweep may be defined as a single segment sweep ([*SINGLE SEG SWEEP*] softkey) or an all segment sweep ([*ALL SEGS SWEEP*] softkey). The frequency list table can be entered and modified with [*EDIT LIST*].

*Next Menu Page 33*

**POWER SWEEP** Sweeps power at a single frequency. That frequency is set with [*CW FREQ*]. Power sweep is used to characterize power sensitive networks.


**CW TIME** Tunes the analyzer to a single frequency and displays the data versus time. The frequency is set with [*CW FREQ*]. With option 010 (time domain), the analyzer can translate this data to the frequency domain.

**EDIT LIST** Allows the user to create or modify the frequency list table.

*Next Menu Page 33*

**RETURN** Returns to the previous menu.

# MENU

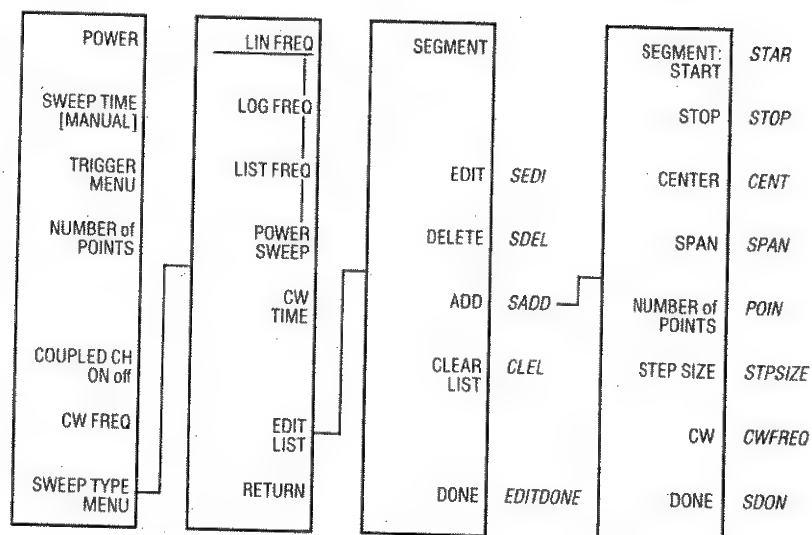

## List Frequency Mode


List frequency mode customizes the sweep to your specific measurement needs. You can define either the specific frequencies to be measured, or a series of subsweeps with the span and number of points desired. Once the list has been defined, the analyzer will measure according to the list. Displayed is a single trace, the composite data of all the sweep segments or a single sweep segment.

List frequency mode works with all the display functions, including calibration, markers, limit testing, averaging, trace memory, and vector trace math.

The list frequency table is entered through **[EDIT LIST]**. Enter a series of up to 30 sweep segments. Each segment can contain a single point or multiple points. The total number of points in the frequency list table cannot exceed 1632.

The default for list frequency sweep is a sweep of all the segments in the frequency list table. To sweep a single segment, select the **[SINGLE SEG SWEEP]** softkey in the list frequency menu. Different segments can be swept by changing the segment number using the front panel rotary knob, the step keys, or the keypad.

MKR

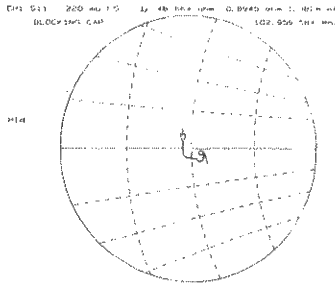

## Markers

The analyzer markers provide numerical readout of trace data. The markers are controlled from the [MKR] key, and the active functions involving markers are controlled from [MKR FCTN].

In addition to turning markers on and off, [MKR] provides extensive control of the markers and the marker values.

## Delta Markers

This is a relative mode, where the marker values show the position of the active marker relative to the delta reference marker. The delta mode is turned on by defining one of the four markers as the delta reference.

## Marker Zero

Another relative mode, except that the marker values show position relative to a fixed point. Marker zero enters the position of the active marker as the fixed offset. Alternatively, the operator can specify the fixed point with *[FIXED MKR POSITION]*. Marker zero is canceled by turning delta mode off.

## Coupled Markers

Normally, the markers have the same stimulus values on each channel, but they can be uncoupled so that each channel has independent markers.

### Continuous Markers

The analyzer can either place the markers on discrete sampled points, or it can move the markers continuously along the trace by interpolating the marker position.



## Polar Markers

The analyzer can display the marker value as magnitude and phase, or as a real/imaginary pair. **[LIN MKR]** gives linear magnitude and phase, **[LOG MKR]** gives log magnitude and phase. **[Re/Im]** gives the real value first, then the imaginary value.

## Smith Markers

The same selections are available as for polar markers, plus complex admittance and impedance. For complex impedance, the displayed values are real impedance, imaginary impedance, and equivalent capacitance/inductance. The equivalent capacitance/inductance is calculated from the imaginary impedance and frequency. For admittance, the analyzer displays an inverse Smith chart.

**MKR**

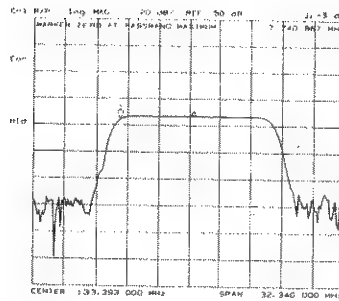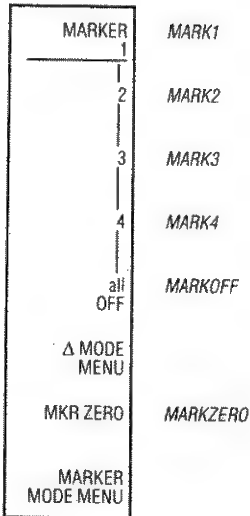

**MARKER 1** Turns on marker 1, and makes it the active marker. The annotation  $\Delta \text{REF} = 1$  indicates that this marker is the delta reference marker.

**2** Turns on marker 2.

**3** Turns on marker 3.

**4** Turns on marker 4.

**all OFF** Turns off all markers.

**Δ MODE MENU** Leads to the delta mode menu.



*Next Menu Page 36*

**MKR ZERO** Zeros the marker values. Once activated, all marker values are the difference between the current position of the active marker and the zero position. Canceled by turning delta mode off.

**MARKER MODE MENU** Allows the user to select special marker modes.

*Next Menu Page 37*

## MKR

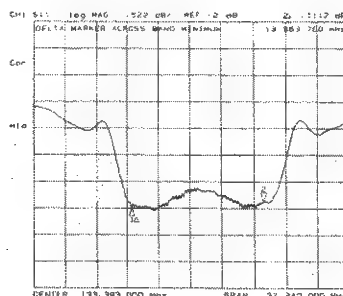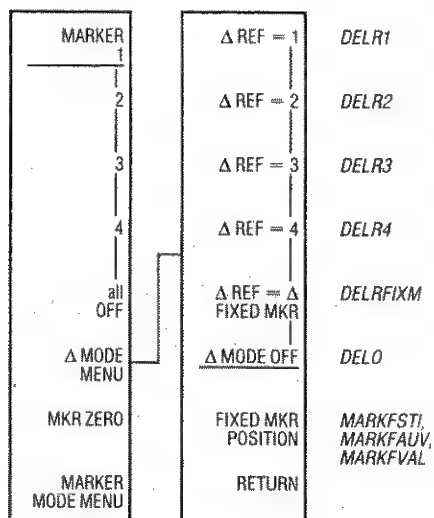

**Δ REF = 1** Marker 1 becomes the delta reference marker. With a delta reference defined, all marker amplitude and stimulus values are the offset between the active marker position and the delta reference position.

**Δ REF = 2** Makes marker 2 the delta reference.

**Δ REF = 3** Makes marker 3 the delta reference.

**Δ REF = 4** Makes marker 4 the delta reference.

**Δ REF = Δ FIXED MKR** Turns on a fixed delta reference. A small triangle marks the reference point defined. All marker values are relative to this point. The fixed position is entered with marker zero or [FIXED MKR POSITION].


**Δ MODE OFF** Returns markers to absolute mode.

**FIXED MKR POSITION** Leads to a menu that allows the user to specify fixed marker offsets. Marker zero (page 35) enters the marker position as the fixed marker position.

**RETURN** Returns to the previous menu.



**MKR**

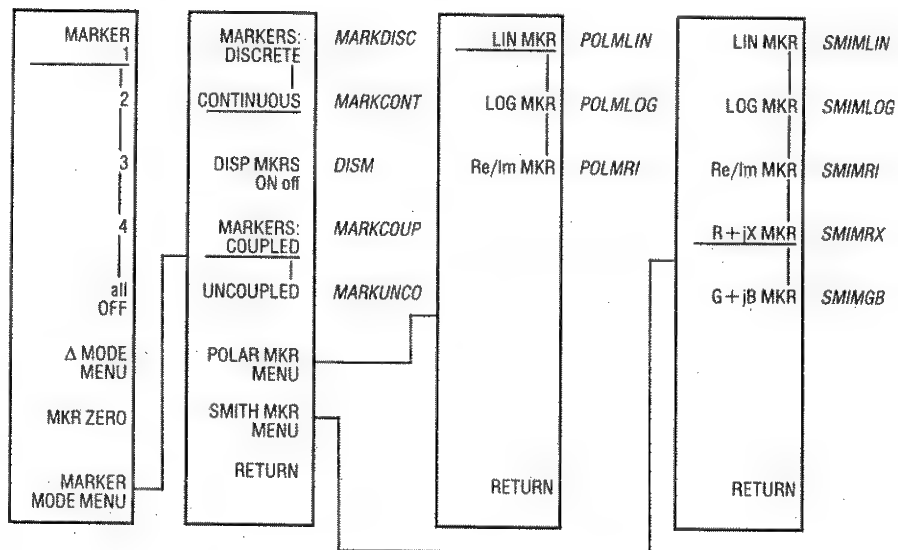

**MARKERS: DISCRETE** Puts markers only on measured points.

**CONTINUOUS** Interpolates the marker placement and values between measured points.

**DISP MKRS ON off** Allow display on CRT and plotting of all markers that are on.

**MARKERS: COUPLED** Puts the markers on the same stimulus values on each channel.


**UNCOUPLED** Makes the markers independent between the channels.

**POLAR MKR MENU** Selects the marker readout format for polar display. The analyzer will display the marker values as linear or log magnitude, or as a real/imaginary pair. See page 34.

**SMITH MKR MENU** Selects the marker readout format for a Smith chart display. Same as polar markers with the additional choices of complex impedance or admittance. See page 34.

**RETURN** Returns to the previous menu.

MKR  
FCTN

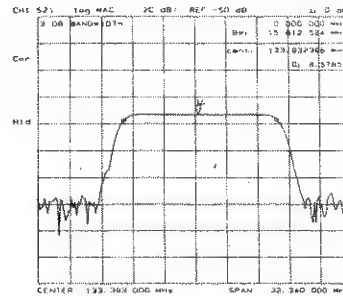

The marker functions use the markers for setting instrument parameters, as search markers, and in calculating various statistics.

## MARKER →

These functions change instrument parameters.

### Marker Search

These functions place the marker at an amplitude-related point on the trace. Turning tracking on makes the analyzer search every new trace for the target point.

### Widths


This analyzes a bandpass or band reject shape on the trace. It calculates center, bandwidth, and Q according to the operator-entered widths value. The widths value is the amplitude value that defines the band start and stop. If a delta reference is on, this function uses it as the reference point of the widths value. For example, with a delta reference marker at the passband maximum and the widths value set to  $-3$  dB, the widths search will find the 3 dB cutoff points of the bandpass and calculate the 3 dB bandwidth and Q.

### Statistics (Stats)

Calculates the mean, standard deviation, and peak-to-peak values of the section of the displayed trace between the active marker and the delta reference. If there is no delta reference, the analyzer calculates the statistics for the entire trace.

**MKR  
FCTN**

- MARKER→  
START            MARKSTAR
- MARKER→  
STOP            MARKSTOP
- MARKER→  
CENTER          MARKCENT
- MARKER→  
SPAN            MARKSPAN
- MARKER→  
REFERENCE       MARKREF
- MARKER→  
DELAY           MARKDELA
- MKR SEARCH  
[OFF]
- STATS  
on OFF

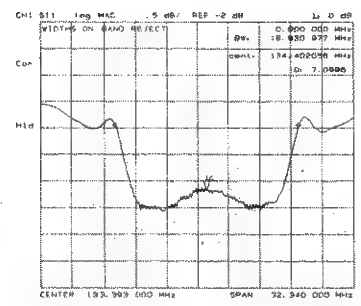


- MARKER → START**      Changes the start stimulus value to the marker stimulus value.
- MARKER → STOP**      Changes the stop stimulus value to the marker stimulus value.
- MARKER → CENTER**      Changes the center stimulus value to the marker stimulus value.
- MARKER → SPAN**      Takes the span between the active marker and the delta reference marker, and makes that the stimulus span.
- MARKER → REFERENCE**      Changes the reference value to the marker amplitude value.
- MARKER → DELAY**      Flattens the phase trace at the marker by adding in electrical delay. See page 43.
- MKR SEARCH [OFF]**      Leads to the search menu, from which the marker placement search parameter is selected.
- STATS on OFF**      Activates the trace statistics function. See page 38.

*Next Menu Page 40*

# MKR FCTN

MARKER→ START	SEARCH: OFF	SEAOFF
MARKER→ STOP	MAX	SEAMAX
MARKER→ CENTER	MIN	SEAMIN
MARKER→ SPAN	TARGET	SEATARG
MARKER→ REFERENCE	WIDTH VALUE	WIDV
MARKER→ DELAY	WIDTHS on OFF	WIDTON, WIDTOFF
MKR SEARCH [OFF]	TRACKING on OFF	TRACKON, TRACKOFF
STATS on OFF	RETURN	

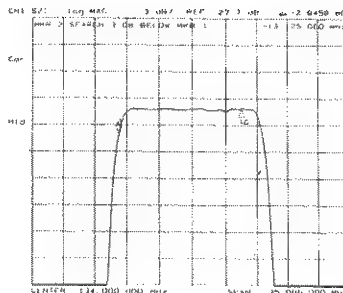

**SEARCH:  
OFF** Turns the active search function off.

**MAX** Moves the marker to the trace maximum.

**MIN** Moves the marker to the trace minimum.

**TARGET** Moves the marker to the specified amplitude value on the trace. Leads to a menu with search right and search left options to resolve multiple solutions.

**WIDTH  
VALUE** The amplitude parameter for the widths search. See page 38.

**WIDTHS  
on OFF** Calculates the center stimulus, bandwidth, and Q of a bandpass or band reject shape on the trace. The width value is the amplitude search parameter that defines the passband or reject band.

**TRACKING  
on OFF** Makes the analyzer track the search with each new sweep.

**RETURN** Returns to the previous menu.

**SAVE**

**RECALL**

RE-SAVE REG 1	SAVE1
RE-SAVE REG 2	SAVE2
RE-SAVE REG 3	SAVE3
RE-SAVE REG 4	SAVE4
RE-SAVE REG 5	SAVE5
CLEAR REGISTER	
TITLE REGISTER	
STORE TO DISK	

RECALL REG 1	RECA1
RECALL REG 2	RECA2
RECALL REG 3	RECA3
RECALL REG 4	RECA4
RECALL REG 5	RECA5
RECALL PRST STATE	PRES
LOAD FROM DISK	

## Instrument State Storage/Retrieval


The analyzer will store complete instrument states for later retrieval, and has five internal registers as well as direct disk access for this purpose. Because instrument states can be of varying complexities, it is possible to fill the available memory with less than five states. Also, it is possible to fill memory with instrument states and prevent such memory-intensive functions as 2-port measurement calibration, time domain (option 010), or 1601 points.

The size of an instrument state is proportional to the number of points in the sweep, and dependent on the use of calibration, limit testing, and list frequencies. If these functions are on when the instrument state is saved, the information used by these functions is also saved.

Certain memory-intensive sets of information, such as calibration data, trace data, and trace memory, are stored in volatile memory. Volatile memory is lost whenever power is turned off, whereas the short-term memory lasts several days with the power off.

The menus indicate whether a register has been saved or not. If a register has not been saved, the save softkey is **[SAVE]**, and if it has, the save softkey will read **[RE-SAVE]**. Similarly, if a register has not been saved, there is no recall or clear option given for that register.

## SAVE

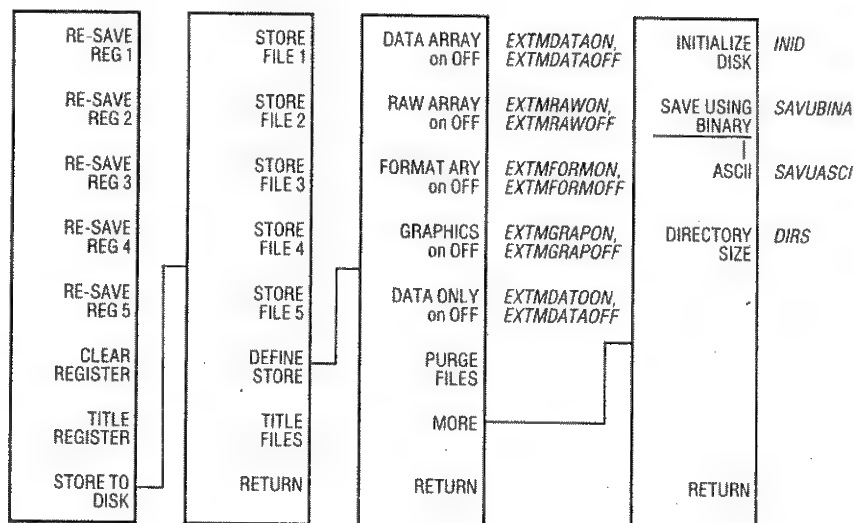

The disk access functions are controlled through the **[STORE TO DISK]** and **[LOAD FROM DISK]** menus under the **[SAVE]** and **[RECALL]** keys, respectively. In addition to the complete instrument state, some information that is not included in the internal registers can be stored on disk.

The additionally stored information is selected using the **[DEFINE STORE]** menu. Measurement data can be saved in several forms: as data, raw data, or formatted data. Most commonly, the data array is stored. The raw data is the data prior to error correction, and formatted data is the data after such formatting as electrical delay, time domain, smoothing, and trace math. Aside from measurement data, the user graphics, which must be entered with a computer, can also be saved.


To store a state on disk, first title a file using the **[TITLE FILES]** menu. Then store the current instrument state on disk by selecting the file under the **[STORE TO DISK]** menu.

To load a file from disk, press **[RECALL]** **[LOAD FROM DISK]** **[READ FILE TITLES]**, and select the desired file. If there are more than five files on the disk, press **[READ FILE TITLES]** again and the analyzer will display the next five files on the disk.

The analyzer must be in either system controller or pass control mode, and the correct disk unit and volume number must be set in the **[LOCAL]** menu. The disk unit number selects a drive in a dual or Winchester disk drive. The volume number specifies which volume is to be accessed in hard disk drives. If a flexible disk drive is being used, the volume number should be set to zero.

**SCALE  
REF**

<b>AUTO SCALE</b>	<i>AUTO</i>
<b>SCALE/DIV</b>	<i>SCAL</i>
<b>REFERENCE POSITION</b>	<i>REFP</i>
<b>REFERENCE VALUE</b>	<i>REFV</i>
<b>MARKER → REFERENCE</b>	<i>MARKREF</i>
<b>MARKER → DELAY</b>	<i>MARKDELA</i>
<b>ELECTRICAL DELAY</b>	<i>ELED</i>
<b>PHASE OFFSET</b>	<i>PHAO</i>

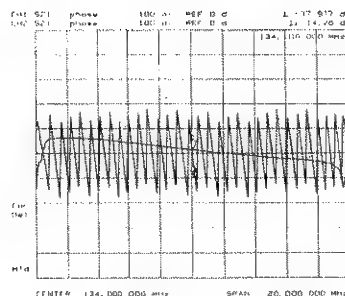

- AUTO SCALE** Finds the trace and scales it so that it fits on the graticule.
- SCALE/DIV** Changes the trace scaling.
- REFERENCE POSITION** Moves the reference line up and down the graticule, 0 being the bottom of the graticule, and 10 the top.
- REFERENCE VALUE** Changes the value of the reference line. In polar and Smith chart formats, the reference value is the value at the outer circle.
- MARKER →  
REFERENCE** Makes the amplitude at the active marker the reference value.
- MARKER →  
DELAY** Sets the electrical delay so that the group delay is 0 at the marker. This flattens the phase trace at the marker.
- ELECTRICAL DELAY** Adds or subtracts electrical time delay from the data. Simulates adding or removing linear phase from a measurement.
- PHASE OFFSET** Adds the specified offset to the measured phase value.

## SYSTEM

SEQUENCING  
MENU

CONTINUE  
SEQUENCE

LIMIT  
MENU

TRANSFORM  
MENU

FREQ RANGE  
3GHz6GHz

HARMONIC  
MEAS

INSTRUMENT  
MODE

SERVICE  
MENU

### Test Sequencing Function

Sequencing allows any list functions to be executed automatically with a single key-stroke. The sequences can be entered from the front panel, read from an external disk, or down loaded over HP-IB from an external controller.

### Limit Testing

The analyzer's limit testing feature provides pass/fail testing in frequency, time, or power domains.

#### Time Domain (Option 010)

The analyzer uses the inverse Fourier transform to calculate the time domain step and impulse responses of a DUT. Furthermore, it allows the user to position a time gate over the data, which it then applies directly to frequency domain data. The transform can also convert CW time domain data to frequency domain for baseband analysis.

#### Frequency Range (Option 006)

6 GHz measurement capability requires a HP 8753C (Option 006), and a HP 85047A S-parameter test set. This softkey toggles between operation in the 300 kHz to 3 GHz and 3 MHz to 6 GHz frequency ranges.

#### Harmonic Measurements (Option 002)

Harmonic measurements mode enables the analyzer's receivers to measure the 2nd or 3rd order harmonic response of a DUT as its source sweeps the fundamental frequency range. Option 006 is required for 2nd and 3rd harmonic frequencies from 3 to 6 GHz.

#### Instrument Mode

Allows the user to select between network analyzer, external source, tuned receiver, or frequency offset modes of operation.



## SYSTEM

SEQUENCE  
SEQ1

SEQUENCE  
SEQ2

SEQUENCE  
SEQ3

SEQUENCE  
SEQ4

SEQUENCE  
SEQ5

SEQUENCE  
AUTO

PAUSE TO  
SELECT

RETURN

### TEST SEQUENCING

#### MODIFY

- INSERT - Any function is inserted after cursor.
- DELETE - BACK SP deletes line at cursor.
- STEP - Use ARROW keys or RPN. ARROW up does the function at the cursor and moves list up. ARROW down only moves list down.
- END - Press DONE MODIFY in SEQUENCE MENU.

#### RUN

- START - Press DO SEQUENCE in SEQUENCE MENU.
- KEYS - All front panel keys except LOCAL are locked out until sequence stops.
- STOP - Press LOCAL to stop a running sequence.
- PAUSE - Press CONTINUE SEQUENCE in SYSTEM MENU to restart a paused sequence.

Only sequence 6 is saved when instrument is turned off.

For more information, see Test Sequencing chapter in System Operating and Programming Manual.

Select a softkey to start modifying a sequence.

## Test Sequencing Function


The Test Sequencing Function allows you to combine a series of features such as limit testing, harmonic measurements, and marker functions, with if/then decision capabilities into a test executable by a single keystroke.

Creating a test sequence is virtually identical to making a manual measurement using the front panel. Once you have entered sequencing mode all you need to do is make the desired measurement. The analyzer will record the keystrokes it took to do so, storing them where they can be called up and repeated with a single keystroke. Test sequences may be stored in six internal registers, or to an external disk.

The analyzer allows you to cascade multiple sequences to increase efficiency and reduce test times when performing longer, more elaborate tests.

This feature also allows you to send HP-IB output strings to automatically control external devices, such as signal generators, power supplies, or relay actuators.

## SYSTEM

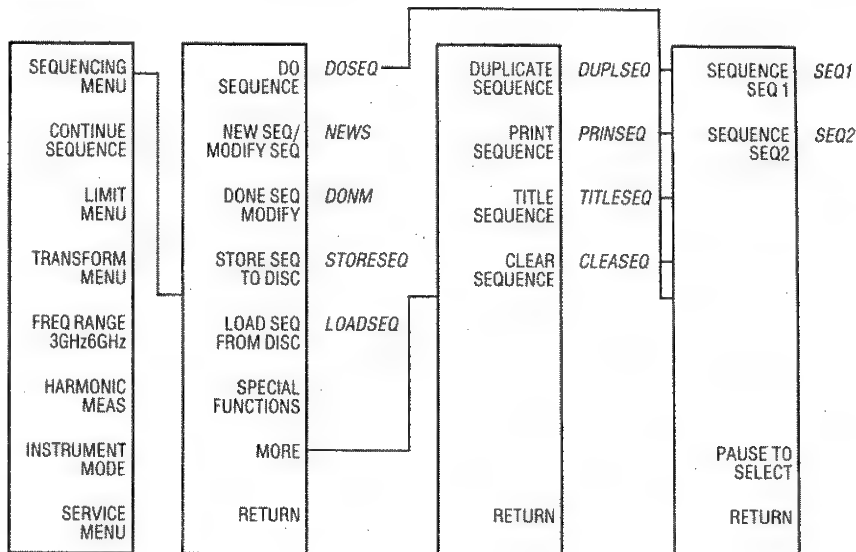

### DO SEQUENCE

Executes a specified sequence.

### NEW SEQ/ MODIFY SEQ

Allows you to create a new or modify an existing sequence. Leads to a set of instructions for creating and modifying a test sequence function.

### DONE SEQ MODIFY

Indicates the completion of modification or creation of a sequence.

### STORE SEQ TO DISC

Stores a sequence to an external disk.

### LOAD SEQ FROM DISC

Loads a sequence from an external disk.

### SPECIAL FUNCTIONS

Leads to the display of titling and decision making capabilities.


### MORE

Leads to more display choices, such as duplicating, printing, titling, and clearing a sequence.

### RETURN

Returns to the previous menu.

# SYSTEM

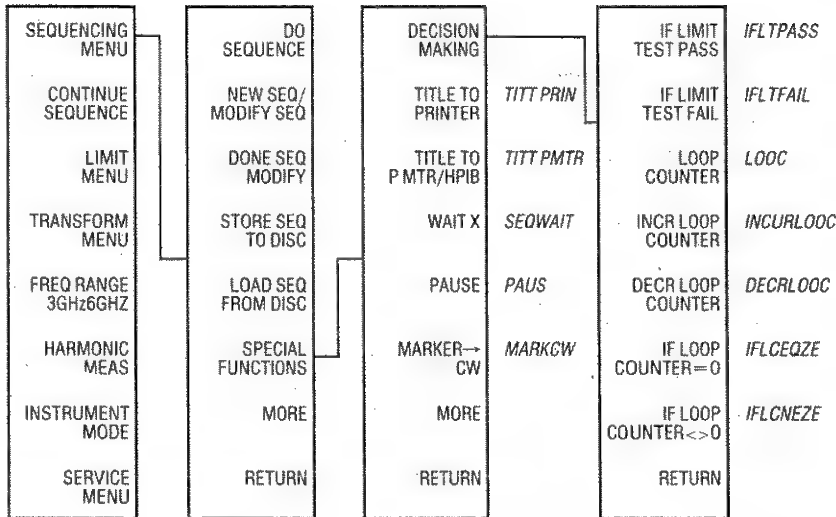

**DECISION MAKING** Leads to a menu that controls pass/fail testing capability and loop counter control.

**TITLE TO PRINTER** Enables you to send a title including letters, numbers, some punctuation, and several control characters to a printer over HP-IB.

**TITLE TO P MTR/HPIB** Enables you to send a command in the form of a title to a HP-IB controllable device.

**WAIT X** This will pause the execution of a sequence for X seconds.


**PAUSE** This command will temporarily stop the execution of a sequence. The keyboard will be freed up allowing the user to change an instrument parameter, or modify an equipment configuration. The sequence can be re-started by pressing the continue or sequence menu keys.

**MARKER -> CW** Move the CW frequency to the marker stimulus value.

**MORE** Leads to more choices (see page 48).

**RETURN** Returns to the previous menu.

## SYSTEM

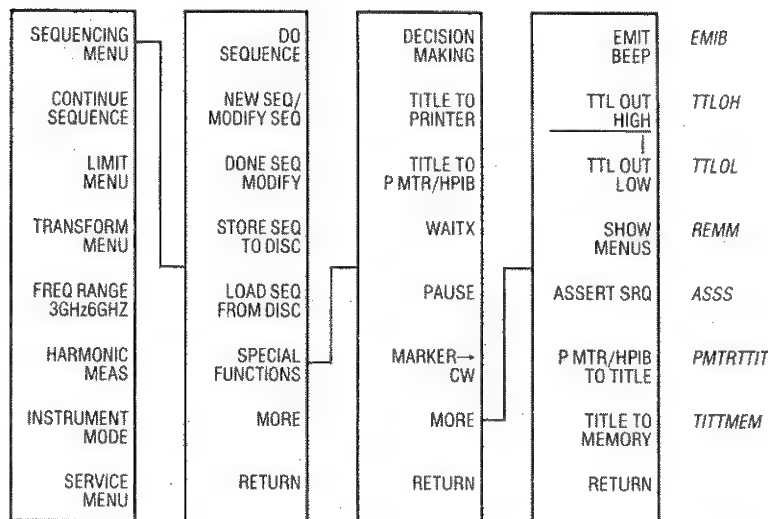

**EMIT BEEP** Emits a beep of fixed tone and duration during the execution of a sequence.

**TTL OUT HIGH** Sets the TTL line, at the back of the HP 85047A test set, high.

**TTL OUT LOW** Sets the TTL line, at the back of the HP 85047A test set, low.

**SHOW MENUS** Enables the recall of menus from within a sequence. This is especially useful when prompting someone for a softkey response in an interactive test situation.


**ASSERT SRQ** Enables the analyzer to signal an external controller that it has completed the execution of a sequence.

**P MTR/HPIB TO TITLE** Enables the analyzer to read a value from an HP-IB instrument. For more information, see the "Test Sequence Function" chapter in the *Operating* manual.

**TITLE TO MEMORY** Store the value read by the [P MTR/HPIB TO TITLE] key into the memory data array.

**RETURN** Returns to the previous menu.

SYSTEM

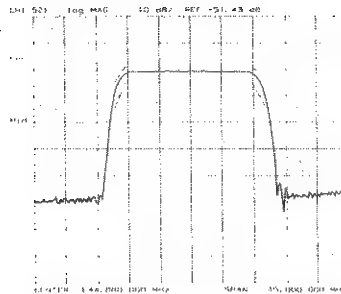

## Limit Testing

Limit testing provides pass/fail testing in frequency or time domains.

Up to 36 limit test segments (18 per channel) can be entered into the limit table. After entry, these segments can then be modified using the **[EDIT LIMIT LINE]** softkey.

The limit table created will be in the current stimulus domain, so that the stimulus values might be frequency or time. The entered stimulus value marks the beginning of the limit segment. The operator enters the limit maximum and minimum at that point. After defining the line, you can select the type of limit segment that is to start at the point.

The upper and lower limits of a sloping line segment connect to the upper and lower limits of the next segment.


The upper and lower limits of a flat line segment extend horizontally to the start of the next segment.

A single point either forms the end of a limit line, or acts as a stand-alone test point.

When limit testing is turned on, the analyzer tests each point that is in a limit test region, and displays a pass or fail message.

## SYSTEM

SEQUENCING MENU	LIMIT LINE on OFF	LIMILINEON, LIMILINEOFF
CONTINUE SEQUENCE	LIMIT TEST on OFF	LIMITESTON, LIMITESTOFF
LIMIT MENU	BEEP FAIL on OFF	BEEPFALON, BEEPFALOFF
TRANSFORM MENU		
FREQ RANGE 3GHz6GHz	EDIT LIMIT LINE	EDITLIML
HARMONIC MEAS		
INSTRUMENT MODE	LIMIT LINE OFFSETS	LIMISTIO, LIMIAMP0, LIMIIMAOF
SERVICE MENU	RETURN	

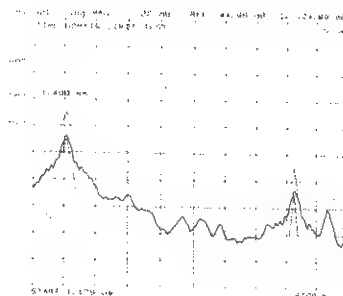

**LIMIT LINE on OFF** Draws the limit lines.

**LIMIT TEST on OFF** Tests each sweep for measured points that are out-of-limit.

**BEEP FAIL on OFF** Sounds the beeper when the limit test fails.


**EDIT LIMIT LINE** Allows the user to enter and modify limit lines.

*Next Menu Page 51*

**LIMIT LINE OFFSETS** Allows the user to offset the limit lines in stimulus and amplitude.

**RETURN** Returns to the previous menu.

# SYSTEM

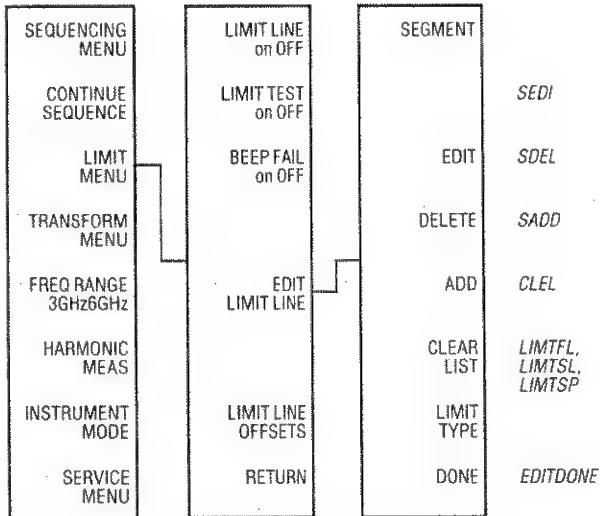

**SEGMENT** Selects the segment to be edited either by entering the segment number, or by using the front panel knob or step keys.

**EDIT** Brings the selected segment up for editing.

**DELETE** Deletes the entry indicated by the pointer.

**ADD** Adds a new entry at the pointer.


*Next Menu Page 52*

**CLEAR LIST** Clears the present list.

**LIMIT TYPE** Allows the user to select the type of limit for the current segment. There are sloping line (SL), flat line (FL), or single point (SP) limit types.

**DONE** Returns to the previous menu.

## SYSTEM

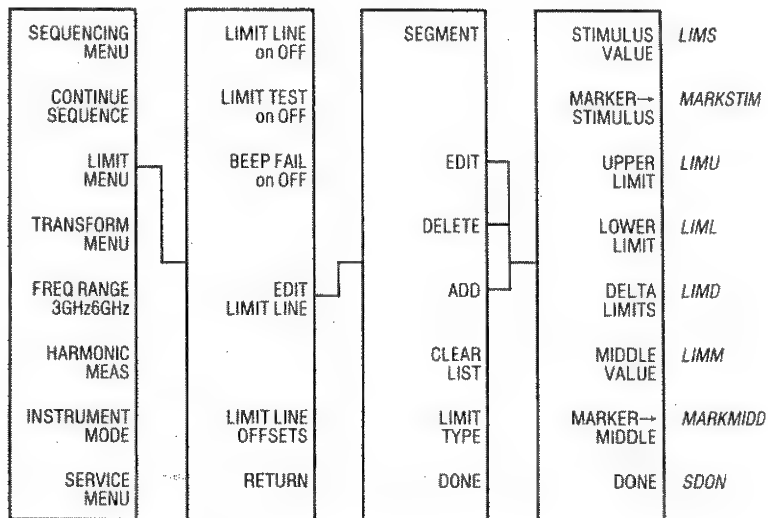

### STIMULUS VALUE

Enters the starting stimulus value of this segment.

### MARKER → STIMULUS

Enters the marker stimulus as the start of this segment.

### UPPER LIMIT

Enters the top limit.

### LOWER LIMIT

Enters the bottom limit.

### DELTA LIMITS

Instead of upper/lower limits, enters amplitude between the the limit lines.

### MIDDLE VALUE

Instead of upper/lower limits, enters the center amplitude between the limit lines.

### MARKER → MIDDLE


Makes the marker amplitude the middle value between the limit lines.

### DONE

Returns to the previous menu.



## SYSTEM

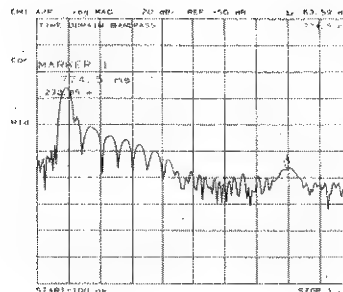

### Time Domain (Option 010)

The analyzer uses the inverse Fourier transform to calculate the time domain step and impulse responses of the DUT. Furthermore, it allows the user to position a time gate over the data, which it then applies directly to the frequency domain data. The transform can also convert CW time domain data to frequency domain for baseband analysis.

#### Window

A true frequency domain impulse or step response would cover all frequencies from zero to infinity. The abrupt limits on the actual frequency sweep cause ringing in time domain. Ringing is reduced by windowing (greater windowing, less ringing,) at the expense of effective impulse width.

#### Demodulation (Demod)

This is intended for use with the CW time to frequency transformation. Amplitude demodulation removes any phase modulation prior to transforming the data. Phase demodulation removes any amplitude modulation. With no demodulation, the transformed data shows the combined amplitude and phase modulation effects.

#### Low Pass Versus Bandpass

Time domain low pass mode simulates traditional TDR measurements. For this to work, however, the frequencies must be set at harmonic intervals. This is done with [SET FREQ]. Bandpass mode avoids this restriction, but is limited to the impulse response. The advantage of bandpass mode is that it allows time domain measurements on highly frequency-selective devices.


#### Gating

The operator can place a time domain bandpass filter on the data, which is called a gate. In effect, the analyzer will remove all responses received before the gate start time and after the gate stop time.

#### Gate Shape

The analyzer allows the user to control the shape of the gate. Minimum gate trades off rapid filter cutoff for less passband ripple.

## SYSTEM

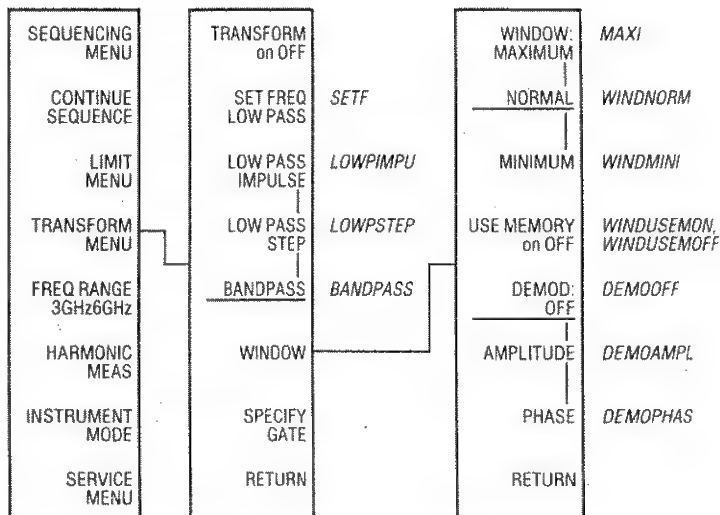

**TRANSFORM on OFF** Turns on the transform and displays the time domain response of a linear frequency sweep, or the frequency domain response of a CW time sweep.

**SET FREQ LOW PASS** Sets the frequencies to harmonic intervals, keeping the number of points the same. Required for low pass mode.

**LOW PASS IMPULSE** Makes the transform display the impulse response. Use the real data format.

**LOW PASS STEP** Makes the transform display the step response of the DUT. Use the real data format.

**BANDPASS** Makes the transform display the impulse response. Can operate with band-limited frequency data. The most useful data formats are linear and log magnitude.


**WINDOW** Places a window over the frequency domain data to minimize the effect of abrupt frequency cutoff at the ends of the sweep. Also controls amplitude and phase demodulation.

**SPECIFY GATE** Allows you to place a time gate over both frequency and time domain data. The gate shape is selectable.

*Next Menu Page 55*

**RETURN** Returns to the previous menu.

# SYSTEM

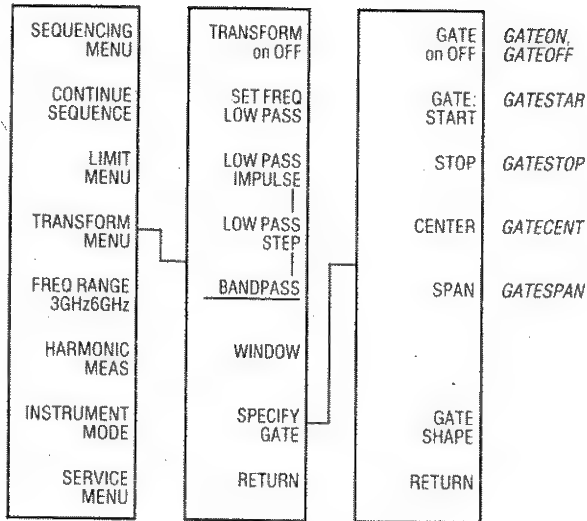

**GATE on OFF** Turns the gate on and off. Although the gate is set in the time domain, it is actually applied to the frequency domain data.

**GATE: START** Sets the start time of the gate.

**STOP** Sets the stop time of the gate.



**CENTER** Sets the center of the gate.

**SPAN** Sets the span of the gate.

**GATE SHAPE** Allows the user to trade a very flat gate passband at maximum gate shape with very fast cutoff at minimum gate.

**RETURN** Returns to the previous menu.


## SYSTEM

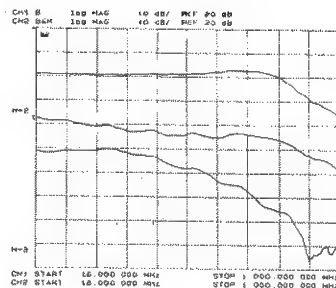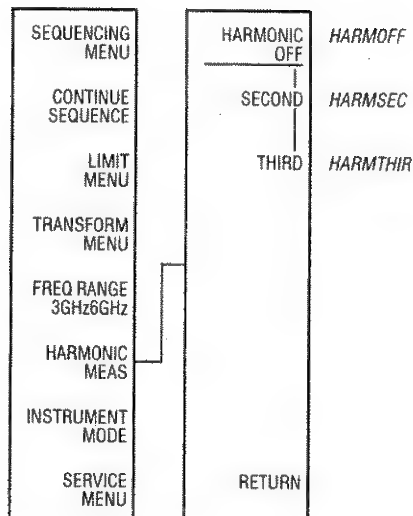

### Harmonic Measurements (Option 002)

- HARMONIC OFF** Turns off harmonic measurement mode so that the receiver is no longer tracking over a harmonic of the source frequency range.
- SECOND** Enables the receiver to track the second harmonic of the source's fundamental frequency range. This measurement is made on a non-ratio basis.
- THIRD** Enables the receiver to track the third harmonic of the source's fundamental frequency range. This measurement is made on a non-ratio basis.
- RETURN** Returns to the previous menu.

## SYSTEM

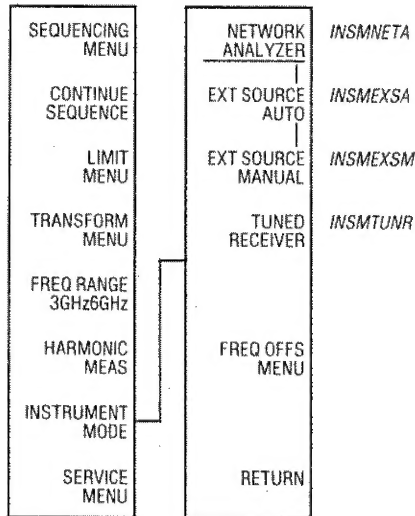

**NETWORK ANALYZER** This is the default mode.

**EXT SOURCE AUTO** Enables the analyzer to phaselock to an external CW frequency. Ext source auto will search the frequency range around the CW frequency for a signal to lock to.

**EXT SOURCE MANUAL** Enables the analyzer to phaselock to an external CW frequency. Ext source manual will try to phaselock to the CW frequency set up by the user. This manual mode enables the analyzer to operate at a much faster rate than in auto mode.

**TUNED RECEIVER** This mode of operation will tune the analyzer to a user specified frequency. Because the instrument bypasses all phaselock routines this mode of operation is very fast but requires the use of very stable source so that signals to be measured will fall within the IF bandwidth of the instrument. This typically requires a synthesizer that can supply an external reference to the analyzer.

**FREQ OFFS MENU** This feature allows the frequency of the analyzer's source to be offset above or below its receiver by a constant value.

**RETURN** Returns to the previous menu.

# Index

## -A-

Active entry area	7
Addresses	26
Analog in	30
Aperture	9
Arbitrary sweep	33
Attenuator control	30
Autoscale	43
Auxiliary input	28
Averaging	8
[AVG]	9

## -B-

Bandpass	53
Beeper	19

## -C-

[CAL]	12
Calibration kit	10
Calibration	10
[CENTER]	3
Clear registers	41
Continuous markers	37
Conversion	27
[COPY]	16
Correction	10
Coupled channels	29
Coupled markers	37
CRT title	19
CW Freq	29
CW time	32

## -D-

Decision making	47
Default plot setup	16
Define sweep	33
Delay, electrical	43
Delay, group	24
Delta markers	36
Demodulation	53
Directivity	11
Disc	42
Discrete markers	37
[DISPLAY]	18
Display layout	7
Display title	19
Display warnings	6
Do sequence	46
Dual channel	18

## -E-

Electrical delay	43
Entry area	3
Error correction	10
Error messages	6
Extensions	15
External disc	42
External source mode	57
External trigger	31

## -F-

Fixed marker offset	36
Focus	19
[FORMAT]	24
Frequency blank	19
Frequency list	33
Frequency offset mode	57
Full 2-port calibration	13

## -G-

Gate shape	55
Gating	53
Group delay	24

## -H-

Harmonic Measurements	56
HP-IB	25
HP-IB mode	26
Hold	31

## -I-

IF bandwidth	9
Imaginary	24
Impulse	54
Input ports	28
Instrument modes	57
Instrument state	41
Intensity	19
Interpolated markers	37
Inverted Smith	34
Isolation	11

<b>-L-</b>	
Limit lines	49
Limit testing	49
Line stretcher	43
Linear magnitude	20
Linear sweep	32
List frequency	33
List values	16
Load match	11
[LOCAL]	26
Log frequency sweep	32
Log magnitude	24
Loss sensor list	14
Low pass	53

<b>-M-</b>	
Magnitude	24
Marker equals	39
Marker functions	38
Marker offsets	36
Marker search	40
Marker statistics	39
Marker →	39
Marker zero	35
Markers	34
Max	40
[MEAS]	27
Memory	18
[MENU]	29
Message area	7
Min	40
[MKR]	35
[MRK FCTN]	39
Modify calibration kit	10
Modify sequence	46

<b>-N-</b>	
Noise reduction	8
Number of groups	31
Number of points	29

<b>-O-</b>	
Offset value	57
One-path, 2-port	13
Operating parameters	16
Output power	29

<b>-P-</b>	
Pass control	26
Pen speed	17
Pens	16
Phase	24
Plot	16
Plot quadrant	16
Plot scale	17
Plot speed	17
Points	29
Polar	24
Polar markers	37
Port extensions	15
Port ratio	27
Power	29
Power meter calibration	14
Power slope	30
Power sweep	32
[PRESET]	5
Print	16

<b>-Q-</b>	
Quadrant	16

<b>-R-</b>	
Real	24
[RECALL]	42
Reference position	43
Reference value	42
Response	4
Response calibration	13
Response/isolation	13
RF power	30

<b>-S-</b>	
S-parameters	28
S11 1-port calibration	13
S22 1-port calibration	13
[SAVE]	41
[SCALE REF]	43
Search	40
Second Harmonic	56
Sensor Cal Factor	14
Set frequencies	54
Single sweep	31
Slope	30
Smith chart	24
Smith markers	37
Smoothing	8
Soft key area	7
Source control	29
Source match	11
[SPAN]	3
Split display	19
Statistics	39
[START]	3
Stimulus	3
Stimulus couple	29
[STOP]	3
Sweep time	29
Sweep trigger	31
Sweep type	32
SWR	24
System controller	26
[SYSTEM]	5

<b>-T-</b>	
Table, list sweep	32
Talker/listener	26
Target	40
Tests sequence function	45
Test set attenuation	30
Third harmonic	56
Time domain (010)	53
Title	19
Trace math	18
Trace maximum	40
Trace memory	18
Trace minimum	40
Tracking	40
Transform	54
Trigger	31
Tuned receiver mode	57

<b>-U-</b>	
Uncoupled markers	37
Use pass control	26
<b>-V-</b>	
Vector trace math	18
Velocity factor	15
<b>-W-</b>	
Warnings	6
Widths	40
Window	54
<b>-Z-</b>	
Z0	15